

# ELISA for Monkey Apolipoprotein E

Product Code: 3712M-1H-6

---

CONTENTS, development kit for 6 plates:

**Vial 1 (red top)**

Monoclonal antibody E981 (300  $\mu$ l)

Concentration: 0.5 mg/ml

**Vial 2 (yellow top)**

Biotinylated monoclonal antibody E887 (150  $\mu$ l)

Concentration: 0.5 mg/ml

**Vial 3 (white top)**

Streptavidin-Horseradish peroxidase (80  $\mu$ l)

**Vial 4**

Recombinant apoE3 standard (5  $\mu$ g)

To ensure total recovery of stated quantity, vials have been overfilled.

**STORAGE:**

Shipped at ambient temperature. On arrival box 1 should be stored refrigerated at 4-8°C and box 2 should be stored frozen at -20°C.

# General


**Intended use:** For quantitative determination of native and recombinant Apolipoprotein E in serum/plasma samples and cell culture supernatants.

**Serum/plasma samples:** The mAbs will recognize apoE only in the presence of non-ionic detergents at a concentration of 0.01-0.5%. Avoid vortex in the presence of detergent. We recommend the use of Assay buffer (product code: 3652-J2) for dilution of samples, standard and detection antibody. The buffer also prevents false positive read-outs which may be caused by interference of heterophilic antibodies commonly found in plasma and serum. Serum/plasma samples containing EDTA, citrate or heparin may be used. However, heparin containing samples will give higher apoE values due to displacement of proteoglycan bound apoE. Please contact Mabtech for further information.

**Reagents:** Antibodies are supplied in sterile-filtered (0.2  $\mu\text{m}$ ) PBS with sodium azide (0.02%). Streptavidin-HRP is supplied in PBS with 1% BSA and 0.15% Kathon CG.

**Standard range:** 0.1-10 ng/ml

**Standard calibration:** No international standard exists for calibration.

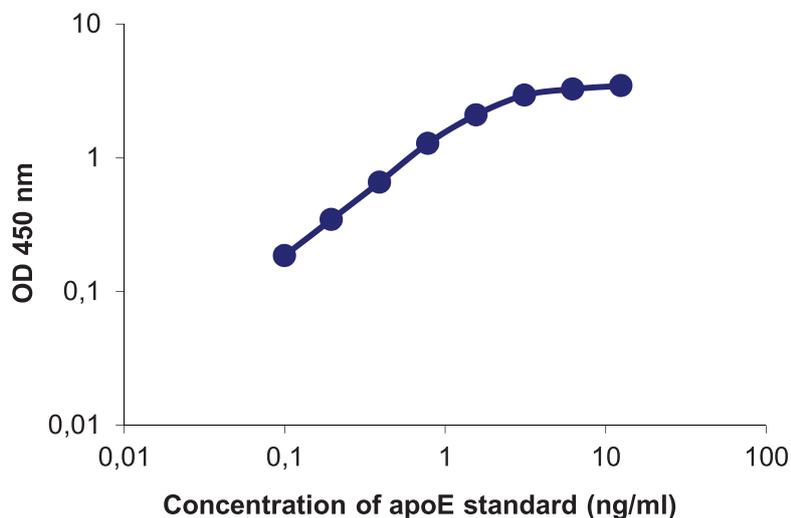

# Guidelines for Monkey Apolipoprotein E ELISA

- Day 1**
1. Coat a high protein binding ELISA plate with mAb E981, diluted to 2  $\mu\text{g}/\text{ml}$  in PBS, pH 7.4, by adding 100  $\mu\text{l}/\text{well}$ . Incubate overnight at 4-8°C.
- Day 2**
2. Wash twice with PBS (200  $\mu\text{l}/\text{well}$ ).
  3. Block plate by adding 200  $\mu\text{l}/\text{well}$  of PBS with 0.05% Tween 20 containing 0.1% BSA (incubation buffer). Incubate for 1 hour at room temperature.
  4. Wash five times with PBS containing 0.05% Tween.
  5. Prepare apoE standard by reconstituting contents of vial 4 in 1 ml PBS with 0.5 mM DTT and 0.1% BSA, do not stir. It is important to wait 20 minutes before resuspending the liquid. This gives a stock solution of 5  $\mu\text{g}/\text{ml}$  which should be used immediately or stored in aliquots at -20°C for future use. The recommended standard dilutions range from 0.1-10 ng/ml.
  6. Add 100  $\mu\text{l}/\text{well}$  of samples or standards diluted in incubation buffer or Assay buffer for serum/plasma samples and incubate for 1 to 2 hours at room temperature.
  7. Wash as in step 4.
  8. Add 100  $\mu\text{l}/\text{well}$  of mAb E887-biotin at 1  $\mu\text{g}/\text{ml}$  in incubation buffer or Assay buffer for serum/plasma samples. Incubate for 1 hour at room temperature.
  9. Wash as in step 4.
  10. Add 100  $\mu\text{l}/\text{well}$  of Streptavidin-HRP diluted 1:1000 in incubation buffer. Incubate for 1 hour at room temperature. **Please note that sodium azide used in buffers will inhibit HRP activity.**
  11. Wash as in step 4.
  12. Add 100  $\mu\text{l}/\text{well}$  of appropriate substrate solution.
  13. Measure the optical density in an ELISA reader after suitable developing time. If required stop the reaction first.

**NOTE; for research use only.**

MABTECH shall not be liable for the use or handling of the product or for consequential, special, indirect or incidental damages therefrom.



MABTECH AB  
Box 1233  
SE-131 28 Nacka Strand  
Sweden  
Tel: +46 8 716 27 00  
Fax: +46 8 716 27 01  
E-mail: [mabtech@mabtech.com](mailto:mabtech@mabtech.com)  
[www.mabtech.com](http://www.mabtech.com)

MABTECH Inc  
M.E.B. 220  
3814 West Street  
Cincinnati, OH 45227  
USA  
Tel: +1 513 871 4500  
Fax: +1 513 871 7353  
E-mail: [mabtech.usa@mabtech.com](mailto:mabtech.usa@mabtech.com)

MABTECH AB Büro Deutschland  
Germany  
Tel: +49 40 4135 7935  
Fax: +49 40 4135 7945  
E-mail: [mabtech.de@mabtech.com](mailto:mabtech.de@mabtech.com)

2013-01-24

Developed and manufactured by MABTECH AB, Sweden, whose quality management system complies with the following standards:



MABTECH AUSTRALIA Pty Ltd  
resolvingIMAGES  
Unit 22, 196 Settlement Road  
Thomastown Victoria 3074  
Australia  
Tel: +61 3 9466 4007  
Fax: +61 3 9466 4003  
E-mail: [mabtech.au@mabtech.com](mailto:mabtech.au@mabtech.com)

MABTECH AB Bureau de liaison France  
BP 255, 1300 route des Crêtes  
06905 Sophia Antipolis  
France  
Tel: +33 (0)4 92 38 80 70  
Fax: +33 (0)4 92 38 80 71  
E-mail: [mabtech.fr@mabtech.com](mailto:mabtech.fr@mabtech.com)