

# PRODUCT INFORMATION & MANUAL

## Rat IL-17A Platinum ELISA

***BMS635 / BMS635TEN***

Enzyme-linked Immunosorbent Assay for  
quantitative detection of rat IL-17A.

For research use only.

Not for diagnostic or therapeutic procedures.



### *Rat IL-17A Platinum ELISA*

#### **North America**

Technical Support:

Research Products:  
888.810.6168  
858.642.2058  
tech@eBioscience.com

Clinical Products:  
877.726.8559  
858.642.2058  
tech@eBioscience.com

Customer Service:

888.999.1371  
858.642.2058  
info@eBioscience.com

Fax:

858.642.2046

#### **Europe/International\***

Technical Support:

+43 1 796 40 40-120  
tech@eBioscience.com

Customer Service:

+43 1 796 40 40-304  
info@eBioscience.com

Fax:

+43 1 796 40 40-400



Bender MedSystems GmbH  
Campus Vienna Biocenter 2  
1030 Vienna, Austria  
www.eBioscience.com

\* Customers outside North America and Europe may contact their eBioscience distributor listed on our website at [www.eBioscience.com/distributors](http://www.eBioscience.com/distributors).

## TABLE OF CONTENTS

|    |  |    |
|----|--|----|
| 1  | Intended Use                                 | 3  |
| 2  | Summary                                      | 3  |
| 3  | Principles of the Test                       | 4  |
| 4  | Reagents Provided                            | 6  |
| 5  | Storage Instructions – ELISA Kit             | 8  |
| 6  | Specimen Collection and Storage Instructions | 8  |
| 7  | Materials Required But Not Provided          | 9  |
| 8  | Precautions for Use                          | 10 |
| 9  | Preparation of Reagents                      | 12 |
| 10 | Test Protocol                                | 17 |
| 11 | Calculation of Results                       | 22 |
| 12 | Limitations                                  | 25 |
| 13 | Performance Characteristics                  | 26 |
| 14 | Ordering Information                         | 31 |
| 15 | Reagent Preparation Summary                  | 32 |
| 16 | Test Protocol Summary                        | 34 |

## 1 Intended Use

The rat IL-17A ELISA is an enzyme-linked immunosorbent assay for the quantitative detection of rat IL-17A. **The rat IL-17A ELISA is for research use only. Not for diagnostic or therapeutic procedures.**

## 2 Summary

A new family of cytokines, Interleukin-17, has recently been defined that reveals a distinct ligand-receptor signaling system. There is high evidence for its importance in the regulation of immune responses. IL-17A was first characterised and six IL-17 family members (IL-17A-F) have subsequently been described. IL-17A, a homodimeric cytokine of about 32 kDa, is largely produced by activated memory T lymphocytes, but stimulates innate immunity and host defense. IL-17A and IL-17F both mobilize neutrophils partly through granulopoiesis and CXC chemokine induction, as well as increased survival locally. IL-17A and IL-17F production by T lymphocytes is regulated by IL-23 independent of T cell receptor activation.

The T help 1 (Th1) and Th2 cell classification has until recently provided the framework for understanding CD4(+) T cell biology and the interplay between innate and adaptive immunity. Recent studies have defined a previously unknown arm of the CD4(+) T cell effector response, the Th17 lineage. This subset of T cells produces interleukin 17, which is highly proinflammatory and induces severe autoimmunity. Whereas IL-23 serves to expand previously differentiated T(H)-17 cell populations, IL-6 and transforming growth factor-beta (TGF-beta) induce the differentiation of T(H)-17 cells from naive precursors.

Increasing evidence shows that IL-17 family members play an active role in inflammatory diseases, autoimmune diseases, and cancer. The IL-17 signaling system is operative in disparate tissues such as articular cartilage, bone, meniscus, brain, hematopoietic tissue, kidney, lung, skin and intestine. Thus, the evolving IL-17 family of ligands and receptors may play an important role in the homeostasis of tissues in health and disease beyond the immune system. Increased levels of IL-17 have been associated with several conditions, including airway inflammation, rheumatoid arthritis, intraperitoneal abscesses and adhesions, inflammatory bowel disease, allograft rejection, psoriasis, cancer and multiple sclerosis.

For literature update refer to **[www.eBioscience.com](http://www.eBioscience.com)**

### 3 Principles of the Test

An anti-rat IL-17A coating antibody is adsorbed onto microwells.

Rat IL-17A present in the sample or standard binds to antibodies adsorbed to the microwells. A biotin-conjugated anti-rat IL-17A antibody is added and binds to rat IL-17A captured by the first antibody.

Following incubation unbound biotin-conjugated anti-rat IL-17A antibody is removed during a wash step. Streptavidin-HRP is added and binds to the biotin-conjugated anti-rat IL-17A antibody.

Following incubation unbound Streptavidin-HRP is removed during a wash step, and substrate solution reactive with HRP is added to the wells.

Figure 1

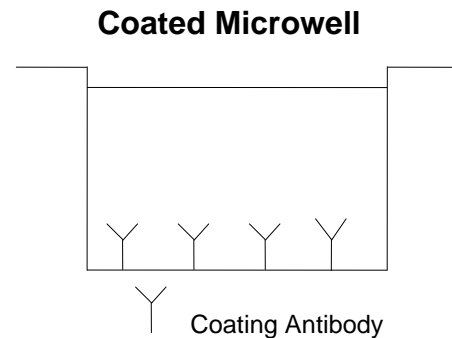


Figure 2

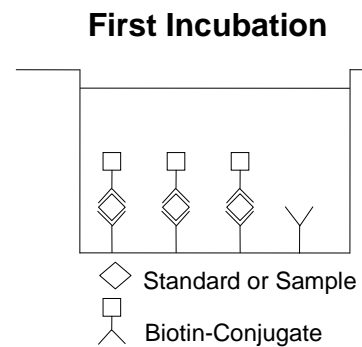


Figure 3



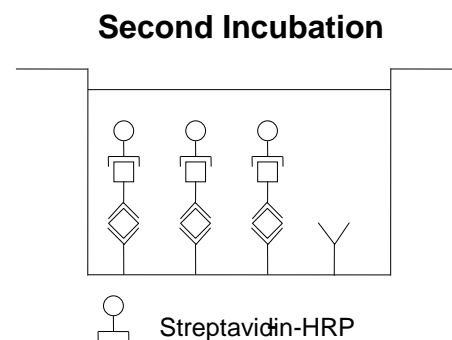


Figure 4

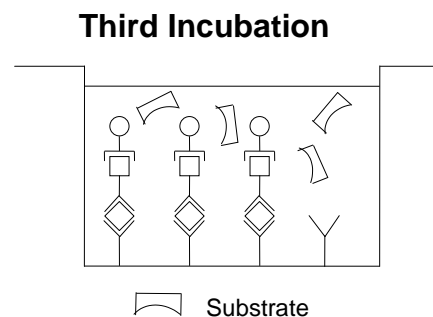

A coloured product is formed in proportion to the amount of rat IL-17A present in the sample or standard. The reaction is terminated by addition of acid and absorbance is measured at 450 nm. A standard curve is prepared 7 rat IL-17A standard dilutions and rat IL-17A sample concentration determined.

Figure 5

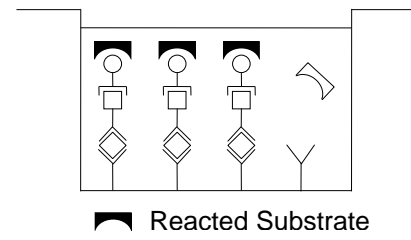

## 4 Reagents Provided

### 4.1 Reagents for rat IL-17A ELISA BMS635 (96 tests)

- 1 aluminium pouch with a **Microwell Plate coated** with monoclonal antibody to rat IL-17A
- 1 vial (70 µl) **Biotin-Conjugate** anti-rat IL-17A monoclonal antibody
- 1 vial (150 µl) **Streptavidin-HRP**
- 2 vials rat IL-17A **Standard** lyophilized, 200 pg/ml upon reconstitution
- 1 bottle (12 ml) **Sample Diluent**
- 1 vial (5 ml) **Assay Buffer Concentrate 20x**  
(PBS with 1% Tween 20 and 10% BSA)
- 1 bottle (50 ml) **Wash Buffer Concentrate 20x**  
(PBS with 1% Tween 20)
- 1 vial (15 ml) **Substrate Solution** (tetramethyl-benzidine)
- 1 vial (15 ml) **Stop Solution** (1M Phosphoric acid)
- 1 vial (0.4 ml) **Blue-Dye**
- 1 vial (0.4 ml) **Green-Dye**
- 1 vial (0.4 ml) **Red-Dye**
- 4 **adhesive Films**

#### 4.2 Reagents for rat IL-17A ELISA BMS635TEN (10x96 tests)

- 10 aluminium pouches with a **Microwell Plate coated** with monoclonal antibody to rat IL-17A
- 10 vials (70 µl) **Biotin-Conjugate** anti-rat IL-17A monoclonal antibody
- 10 vials (150 µl) **Streptavidin-HRP**
- 10 vials rat IL-17A **Standard** lyophilized, 200 pg/ml upon reconstitution
- 10 bottles (12 ml) **Sample Diluent**
- 3 vials (5 ml) **Assay Buffer Concentrate 20x**  
(PBS with 1% Tween 20 and 10% BSA)
- 6 bottles (50 ml) **Wash Buffer Concentrate 20x**  
(PBS with 1% Tween 20)
- 10 vials (15 ml) **Substrate Solution** (tetramethyl-benzidine)
- 10 vials (15 ml) **Stop Solution** (1M Phosphoric acid)
- 6 vials (0.4 ml) **Blue-Dye**
- 6 vials (0.4 ml) **Green-Dye**
- 6 vials (0.4 ml) **Red-Dye**
- 40 **adhesive Films**

## 5 Storage Instructions – ELISA Kit

Store kit reagents between 2° and 8°C.

Immediately after use remaining reagents should be returned to cold storage (2° to 8°C). Expiry of the kit and reagents is stated on labels.

Expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, this reagent is not contaminated by the first handling.

## 6 Specimen Collection and Storage Instructions

Cell culture supernatant, serum and plasma (EDTA, citrate, heparin) were tested with this assay. Other biological samples might be suitable for use in the assay.

Remove serum or plasma from the clot or cells as soon as possible after clotting and separation.

Pay attention to a possible “**Hook Effect**” due to high sample concentrations (see chapter 11).

Samples containing a visible precipitate must be clarified prior to use in the assay. Do not use grossly hemolyzed or lipemic specimens.

Samples should be aliquoted and must be stored frozen at -20°C to avoid loss of bioactive rat IL-17A. If samples are to be run within 24 hours, they may be stored at 2° to 8°C (for sample stability refer to 13.5).

Avoid repeated freeze-thaw cycles. Prior to assay, the frozen sample should be brought to room temperature slowly and mixed gently.



## **7 Materials Required But Not Provided**

- 5 ml and 10 ml graduated pipettes
- 5  $\mu$ l to 1000  $\mu$ l adjustable single channel micropipettes with disposable tips
- 50  $\mu$ l to 300  $\mu$ l adjustable multichannel micropipette with disposable tips
- Multichannel micropipette reservoir
- Beakers, flasks, cylinders necessary for preparation of reagents
- Device for delivery of wash solution (multichannel wash bottle or automatic wash system)
- Microwell strip reader capable of reading at 450 nm (620 nm as optional reference wave length)
- Glass-distilled or deionized water
- Statistical calculator with program to perform regression analysis

## 8 Precautions for Use

- All reagents should be considered as potentially hazardous. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes wash immediately with water. See material safety data sheet(s) and/or safety statement(s) for specific advice.
- Reagents are intended for research use only and are not for use in diagnostic or therapeutic procedures.
- Do not mix or substitute reagents with those from other lots or other sources.
- Do not use kit reagents beyond expiration date on label.
- Do not expose kit reagents to strong light during storage or incubation.
- Do not pipette by mouth.
- Do not eat or smoke in areas where kit reagents or samples are handled.
- Avoid contact of skin or mucous membranes with kit reagents or specimens.
- Rubber or disposable latex gloves should be worn while handling kit reagents or specimens.
- Avoid contact of substrate solution with oxidizing agents and metal.
- Avoid splashing or generation of aerosols.
- In order to avoid microbial contamination or cross-contamination of reagents or specimens which may invalidate the test use disposable pipette tips and/or pipettes.
- Use clean, dedicated reagent trays for dispensing the conjugate and substrate reagent.

- Exposure to acid inactivates the conjugate.
- Glass-distilled water or deionized water must be used for reagent preparation.
- Substrate solution must be at room temperature prior to use.
- Decontaminate and dispose specimens and all potentially contaminated materials as they could contain infectious agents. The preferred method of decontamination is autoclaving for a minimum of 1 hour at 121.5°C.
- Liquid wastes not containing acid and neutralized waste may be mixed with sodium hypochlorite in volumes such that the final mixture contains 1.0% sodium hypochlorite. Allow 30 minutes for effective decontamination. Liquid waste containing acid must be neutralized prior to the addition of sodium hypochlorite.

## 9 Preparation of Reagents

**Buffer Concentrates** should be brought to room temperature and should be diluted before starting the test procedure.

If crystals have formed in the **Buffer Concentrates**, warm them gently until they have completely dissolved.

### 9.1 Wash Buffer (1x)

Pour entire contents (50 ml) of the **Wash Buffer Concentrate** (20x) into a clean 1000 ml graduated cylinder. Bring to final volume of 1000 ml with glass-distilled or deionized water. Mix gently to avoid foaming.

Transfer to a clean wash bottle and store at 2° to 25°C. Please note that Wash Buffer (1x) is stable for 30 days.

Wash Buffer (1x) may also be prepared as needed according to the following table:

| Number of Strips | Wash Buffer Concentrate (20x)<br>(ml) | Distilled Water<br>(ml) |
|------------------|---------------------------------------|-------------------------|
| 1 - 6            | 25                                    | 475                     |
| 1 - 12           | 50                                    | 950                     |

### 9.2 Assay Buffer (1x)

Pour the entire contents (5 ml) of the **Assay Buffer Concentrate** (20x) into a clean 100 ml graduated cylinder. Bring to final volume of 100 ml with distilled water. Mix gently to avoid foaming.

Store at 2° to 8°C. Please note that the Assay Buffer (1x) is stable for 30 days.

Assay Buffer (1x) may also be prepared as needed according to the following table:

| Number of Strips | Assay Buffer Concentrate (20x)<br>(ml) | Distilled Water<br>(ml) |
|------------------|--|-------------------------|
| 1 - 6            | 2.5                                    | 47.5                    |
| 1 - 12           | 5.0                                    | 95.0                    |

### 9.3 Biotin-Conjugate

**Please note that the Biotin-Conjugate should be used within 30 minutes after dilution.**

Make a 1:100 dilution of the concentrated **Biotin-Conjugate** solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

| Number of Strips | Biotin-Conjugate<br>(ml) | Assay Buffer (1x)<br>(ml) |
|------------------|--------------------------|---------------------------|
| 1 - 6            | 0.03                     | 2.97                      |
| 1 - 12           | 0.06                     | 5.94                      |

### 9.4 Streptavidin-HRP

**Please note that the Streptavidin-HRP should be used within 30 minutes after dilution.**

Make a 1:200 dilution of the concentrated **Streptavidin-HRP** solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

| Number of Strips | Streptavidin-HRP<br>(ml) | Assay Buffer (1x)<br>(ml) |
|------------------|--------------------------|---------------------------|
| 1 - 6            | 0.03                     | 5.97                      |
| 1 - 12           | 0.06                     | 11.94                     |

## 9.5 Rat IL-17A Standard

Reconstitute **rat IL-17A standard** by addition of distilled water. Reconstitution volume is stated on the label of the standard vial. Swirl or mix gently to insure complete and homogeneous solubilization (concentration of reconstituted standard = 200 pg/ml). Allow the standard to reconstitute for 10-30 minutes. Mix well prior to making dilutions.

After usage remaining standard cannot be stored and has to be discarded.

**Standard dilutions** can be prepared directly on the microwell plate (see 10.c) or alternatively in tubes (see 9.5.1).

### 9.5.1 External Standard Dilution

Label 7 tubes, one for each standard point.

S1, S2, S3, S4, S5, S6, S7

Then prepare 1:2 serial dilutions for the standard curve as follows:

Pipette 225  $\mu$ l of Sample Diluent into each tube.


Pipette 225  $\mu$ l of reconstituted (concentration of standard = 200.0 pg/ml) into the first tube, labelled S1, and mix (concentration of standard 1 = 100.0 pg/ml).

Pipette 225  $\mu$ l of this dilution into the second tube, labelled S2, and mix thoroughly before the next transfer.

Repeat serial dilutions 5 more times thus creating the points of the standard curve (see Figure 6).

Sample Diluent serves as blank.

Figure 6

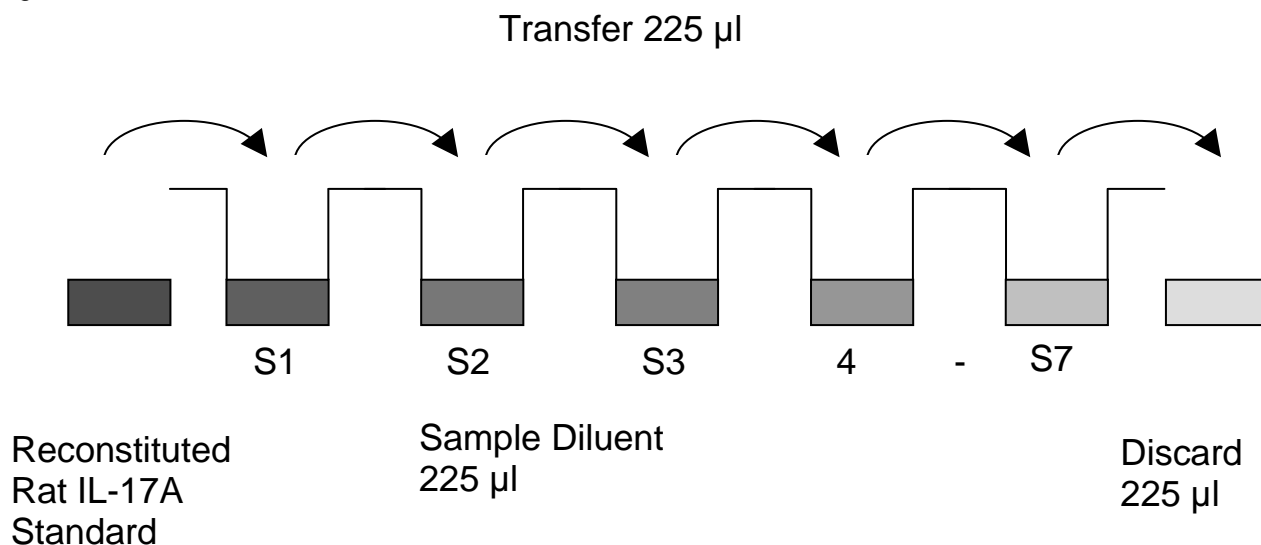

## 9.6 Addition of Colour-giving Reagents: Blue-Dye, Green-Dye, Red-Dye

In order to help our customers to avoid any mistakes in pipetting the Platinum ELISAs, eBioscience offers a tool that helps to monitor the addition of even very small volumes of a solution to the reaction well by giving distinctive colours to each step of the ELISA procedure.

**This procedure is optional**, does not in any way interfere with the test results, and is designed to help the customer with the performance of the test, but can also be omitted, just following the instruction booklet.

Alternatively, the dye solutions from the stocks provided (**Blue-Dye, Green-Dye, Red-Dye**) can be added to the reagents according to the following guidelines:

### 1. Diluent:

Before standard and sample dilution add the **Blue-Dye** at a dilution of 1:250 (see table below) to the appropriate diluent (1x) according to the test protocol. After addition of **Blue-Dye**, proceed according to the instruction booklet.

|                      |                             |
|----------------------|-----------------------------|
| 5 ml Sample Diluent  | 20 $\mu$ l <b>Blue-Dye</b>  |
| 12 ml Sample Diluent | 48 $\mu$ l <b>Blue-Dye</b>  |
| 50 ml Sample Diluent | 200 $\mu$ l <b>Blue-Dye</b> |

- 2. Biotin-Conjugate:** Before dilution of the concentrated Biotin-Conjugate, add the **Green-Dye** at a dilution of 1:100 (see table below) to the Assay Buffer (1x) used for the final conjugate dilution. Proceed after addition of **Green-Dye** according to the instruction booklet: Preparation of Biotin-Conjugate.

|                         |                         |
|-------------------------|-------------------------|
| 3 ml Assay Buffer (1x)  | 30 µl <b>Green-Dye</b>  |
| 6 ml Assay Buffer (1x)  | 60 µl <b>Green-Dye</b>  |
| 12 ml Assay Buffer (1x) | 120 µl <b>Green-Dye</b> |

- 3. Streptavidin-HRP:** Before dilution of the concentrated Streptavidin-HRP, add the **Red-Dye** at a dilution of 1:250 (see table below) to the Assay Buffer (1x) used for the final Streptavidin-HRP dilution. Proceed after addition of **Red-Dye** according to the instruction booklet: Preparation of Streptavidin-HRP.


|                         |                      |
|-------------------------|----------------------|
| 6 ml Assay Buffer (1x)  | 24 µl <b>Red-Dye</b> |
| 12 ml Assay Buffer (1x) | 48 µl <b>Red-Dye</b> |



## 10 Test Protocol

- a. Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running blanks and standards. Each sample, standard, blank and optional control sample should be assayed in duplicate. Remove extra microwell strips from holder and store in foil bag with the desiccant provided at 2°-8°C sealed tightly.
- b. Wash the microwell strips twice with approximately 400 µl **Wash Buffer** per well with thorough aspiration of microwell contents between washes. Allow the Wash Buffer to sit in the wells for about **10 – 15 seconds** before aspiration. Take care not to scratch the surface of the microwells.  
After the last wash step, empty wells and tap microwell strips on absorbent pad or paper towel to remove excess Wash Buffer. Use the microwell strips immediately after washing. Alternatively microwell strips can be placed upside down on a wet absorbent paper for not longer than 15 minutes. **Do not allow wells to dry.**
- c. **Standard dilution on the microwell plate** (Alternatively the standard dilution can be prepared in tubes - see 9.5.1.):  
Add 100 µl of Sample Diluent in duplicate to all **standard wells**.  
Pipette 100 µl of prepared **standard** (see Preparation of Standard 9.5 concentration = 200 pg/ml) in duplicate into well A1 and A2 (see Table 1). Mix the contents of wells A1 and A2 by repeated aspiration and ejection (concentration of standard 1, S1 = 100.0 pg/ml), and transfer 100 µl to wells B1 and B2, respectively (see Figure 7). Take care not to scratch the inner surface of the microwells. Continue this procedure 5 times, creating two rows of rat IL-17A standard dilutions ranging from 100.0 to 1.6 pg/ml. Discard 100 µl of the contents from the last microwells (G1, G2) used.

Figure 7

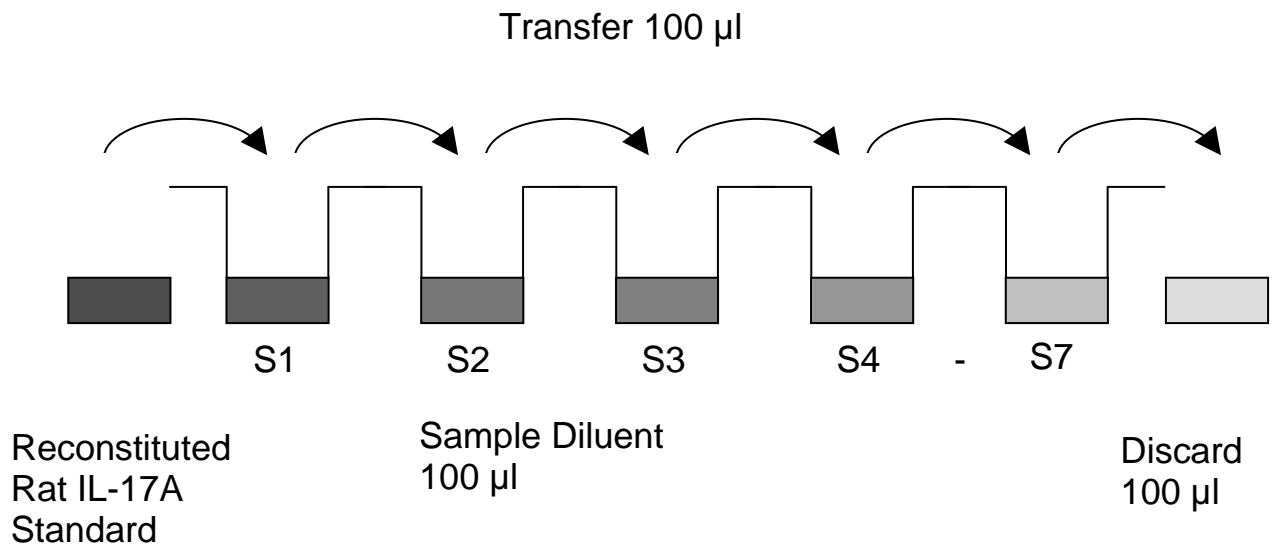

In case of an **external standard dilution** (see 9.5.1), pipette 100 µl of these standard dilutions (S1 - S7) in the standard wells according to Table 1.

Table 1

Table depicting an example of the arrangement of blanks, standards and samples in the microwell strips:

|          | <b>1</b>                    | <b>2</b>                    | <b>3</b> | <b>4</b> |
|----------|-----------------------------|-----------------------------|----------|----------|
| <b>A</b> | Standard 1<br>(100.0 pg/ml) | Standard 1<br>(100.0 pg/ml) | Sample 1 | Sample 1 |
| <b>B</b> | Standard 2<br>(50.0 pg/ml)  | Standard 2<br>(50.0 pg/ml)  | Sample 2 | Sample 2 |
| <b>C</b> | Standard 3<br>(25.0 pg/ml)  | Standard 3<br>(25.0 pg/ml)  | Sample 3 | Sample 3 |
| <b>D</b> | Standard 4<br>(12.5 pg/ml)  | Standard 4<br>(12.5 pg/ml)  | Sample 4 | Sample 4 |
| <b>E</b> | Standard 5<br>(6.3 pg/ml)   | Standard 5<br>(6.3 pg/ml)   | Sample 5 | Sample 5 |
| <b>F</b> | Standard 6<br>(3.1 pg/ml)   | Standard 6<br>(3.1 pg/ml)   | Sample 6 | Sample 6 |
| <b>G</b> | Standard 7<br>(1.6 pg/ml)   | Standard 7<br>(1.6 pg/ml)   | Sample 7 | Sample 7 |
| <b>H</b> | Blank                       | Blank                       | Sample 8 | Sample 8 |

- d. Add 100 µl of **Sample Diluent** in duplicate to the **blank wells**.
- e. Add 50µl of **Sample Diluent** to the **sample wells**.
- f. Add 50 µl of each **sample** in duplicate to the **sample wells**.
- g. Prepare **Biotin-Conjugate** (see Preparation of Biotin-Conjugate 9.3).
- h. Add 50 µl of **Biotin-Conjugate** to all wells.
- i. Cover with an adhesive film and incubate at room temperature (18° to 25°C) for 2 hours, if available on a microplate shaker set at 400 rpm.
- j. Prepare **Streptavidin-HRP** (refer to Preparation of Streptavidin-HRP 9.4).
- k. Remove adhesive film and empty wells. **Wash** microwell strips 4 times according to point b. of the test protocol. Proceed immediately to the next step.
- l. Add 100 µl of diluted **Streptavidin-HRP** to all wells, including the blank wells.
- m. Cover with an adhesive film and incubate at room temperature (18° to 25°C) for 1 hours, if available on a microplate shaker set at 400 rpm.
- n. Remove adhesive film and empty wells. **Wash** microwell strips 4 times according to point b. of the test protocol. Proceed immediately to the next step.
- o. Pipette 100 µl of **TMB Substrate Solution** to all wells.
- p. Incubate the microwell strips at room temperature (18° to 25°C) for about 30 min. Avoid direct exposure to intense light.

**The colour development on the plate should be monitored and the substrate reaction stopped (see next point of this protocol) before positive wells are no longer properly recordable. Determination of the ideal time period for colour development has to be done individually for each assay.**

It is recommended to add the stop solution when the highest standard has developed a dark blue colour. Alternatively the colour development can be monitored by the ELISA reader at 620 nm. The substrate reaction should be stopped as soon as Standard 1 has reached an OD of 0.9 – 0.95.

- q. Stop the enzyme reaction by quickly pipetting 100 µl of **Stop Solution** into each well. It is important that the Stop Solution is spread quickly and uniformly throughout the microwells to completely inactivate the enzyme. Results must be read immediately after the Stop Solution is added or within one hour if the microwell strips are stored at 2 - 8°C in the dark.
- r. Read absorbance of each microwell on a spectro-photometer using 450 nm as the primary wave length (optionally 620 nm as the reference wave length; 610 nm to 650 nm is acceptable). Blank the plate reader according to the manufacturer's instructions by using the blank wells. Determine the absorbance of both the samples and the standards.

**Note: In case of incubation without shaking the obtained O.D. values may be lower than indicated below. Nevertheless the results are still valid.**

## 11 Calculation of Results

- Calculate the average absorbance values for each set of duplicate standards and samples. Duplicates should be within 20 per cent of the mean value.
- Create a standard curve by plotting the mean absorbance for each standard concentration on the ordinate against the rat IL-17A concentration on the abscissa. Draw a best fit curve through the points of the graph (a 5-parameter curve fit is recommended).
- To determine the concentration of circulating rat IL-17A for each sample, first find the mean absorbance value on the ordinate and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the abscissa and read the corresponding rat IL-17A concentration.
- **If instructions in this protocol have been followed samples have been diluted 1:2 (50 µl sample + 50 µl Sample Diluent), the concentration read from the standard curve must be multiplied by the dilution factor (x 2).**
- **Calculation of samples with a concentration exceeding standard 1 may result in incorrect, low rat IL-17A levels. Such samples require further external predilution according to expected rat IL-17A values with Sample Diluent in order to precisely quantitate the actual rat IL-17A level.**
- It is suggested that each testing facility establishes a control sample of known rat IL-17A concentration and runs this additional control with each assay. If the values obtained are not within the expected range of the control, the assay results may be invalid.
- A representative standard curve is shown in Figure 8. This curve cannot be used to derive test results. Each laboratory must prepare a standard curve for each group of microwell strips assayed.

Figure 8

Representative standard curve for rat IL-17A ELISA. Rat IL-17A was diluted in serial 2-fold steps in Sample Diluent. Do not use this standard curve to derive test results. A standard curve must be run for each group of microwell strips assayed.

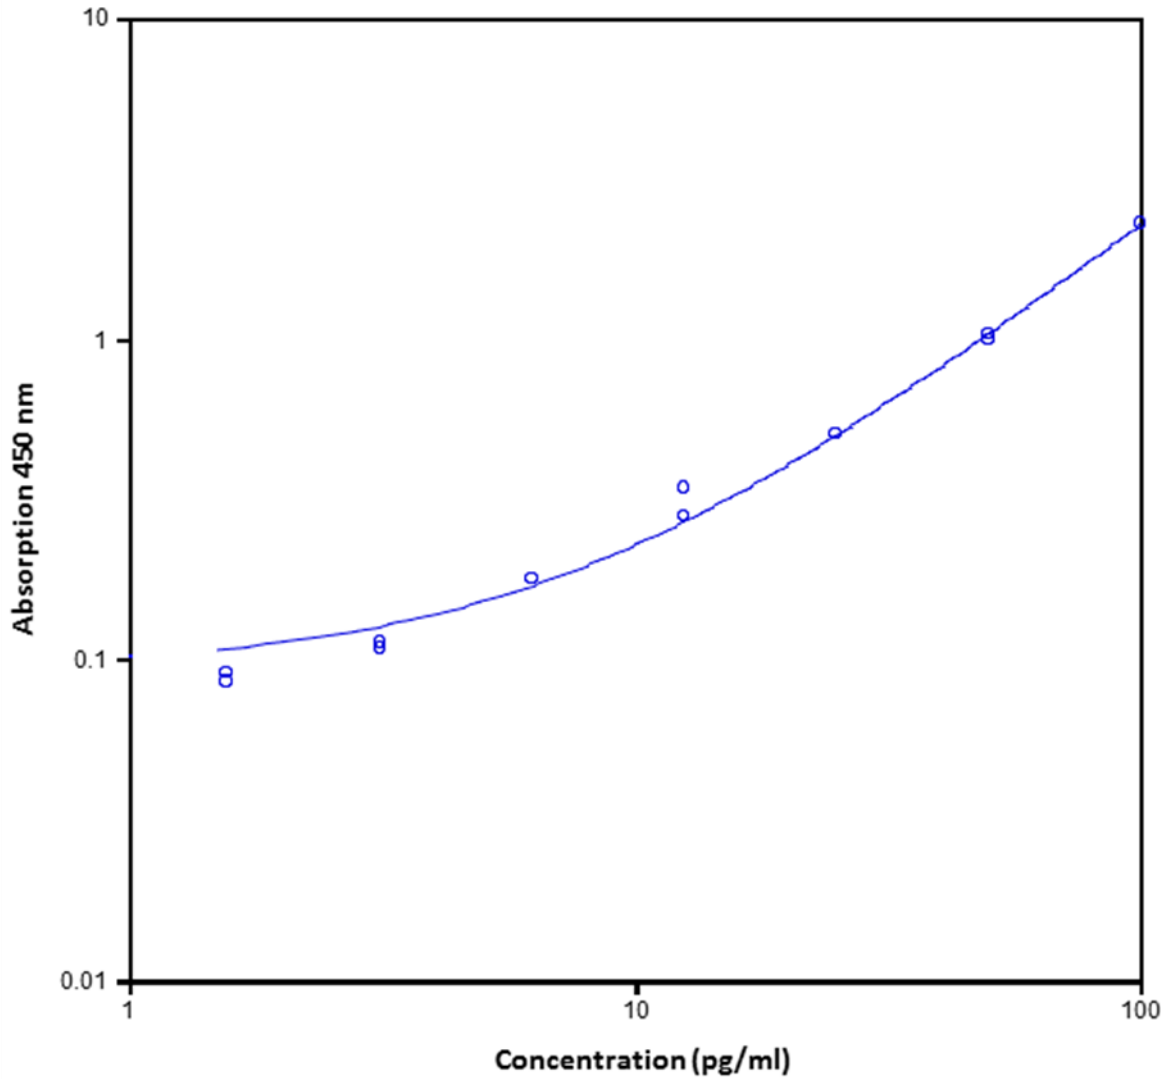


Table 2

Typical data using the rat IL-17A ELISA

Measuring wavelength: 450 nm

Reference wavelength: 620 nm

| Standard | rat IL-17A<br>Concentration<br>(pg/ml) | O.D. at<br>450 nm | Mean<br>O.D. at<br>450 nm | C.V.<br>(%) |
|----------|--|-------------------|---------------------------|-------------|
| 1        | 100.0                                  | 2.297<br>2.300    | 2.299                     | 0.1         |
| 2        | 50.0                                   | 1.037<br>0.999    | 1.018                     | 1.8         |
| 3        | 25.0                                   | 0.509<br>0.506    | 0.508                     | 0.3         |
| 4        | 12.5                                   | 0.344<br>0.282    | 0.313                     | 9.9         |
| 5        | 6.3                                    | 0.178<br>0.180    | 0.179                     | 0.4         |
| 6        | 3.1                                    | 0.114<br>0.108    | 0.111                     | 2.9         |
| 7        | 1.6                                    | 0.091<br>0.086    | 0.089                     | 2.6         |
| Blank    | 0                                      | 0.082<br>0.067    | 0.075                     | 9.8         |

The OD values of the standard curve may vary according to the conditions of assay performance (e.g. operator, pipetting technique, washing technique or temperature effects). Furthermore shelf life of the kit may affect enzymatic activity and thus colour intensity. Values measured are still valid.



## 12 Limitations

- Since exact conditions may vary from assay to assay, a standard curve must be established for every run.
- Bacterial or fungal contamination of either screen samples or reagents or cross-contamination between reagents may cause erroneous results.
- Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.
- Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Empty wells completely before dispensing fresh wash solution, fill with Wash Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

## **13 Performance Characteristics**

### **13.1 Sensitivity**

The limit of detection of rat IL-17A defined as the analyte concentration resulting in an absorbance significantly higher than that of the dilution medium (mean plus 2 standard deviations) was determined to be 1.0 pg/ml (mean of 6 independent assays).

### **13.2 Reproducibility**

#### **13.2.1 Intra-assay**

Reproducibility within the assay was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 7 serum samples containing different concentrations of rat IL-17A. 2 standard curves were run on each plate. Data below show the mean rat IL-17A concentration and the coefficient of variation for each sample (see Table 3). The calculated overall intra-assay coefficient of variation was 8.5%.

Table 3

The mean rat IL-17A concentration and the coefficient of variation for each sample

| Sample | Experiment | Mean rat IL-17A<br>Concentration ( pg/ml) | Coefficient of<br>Variation<br>(%) |
|--------|------------|---|------------------------------------|
| 1      | 1          | 77.62                                     | 4.8                                |
|        | 2          | 78.87                                     | 4.9                                |
|        | 3          | 70.01                                     | 7.8                                |
| 2      | 1          | 48.59                                     | 7.2                                |
|        | 2          | 40.97                                     | 7.4                                |
|        | 3          | 40.80                                     | 19.2                               |
| 3      | 1          | 21.35                                     | 5.3                                |
|        | 2          | 21.05                                     | 5.1                                |
|        | 3          | 18.83                                     | 13.1                               |
| 4      | 1          | 13.56                                     | 3.8                                |
|        | 2          | 10.88                                     | 7.7                                |
|        | 3          | 12.26                                     | 8.3                                |
| 5      | 1          | 70.74                                     | 4.2                                |
|        | 2          | 72.92                                     | 5.7                                |
|        | 3          | 81.50                                     | 4.6                                |
| 6      | 1          | 24.60                                     | 4.8                                |
|        | 2          | 25.17                                     | 6.8                                |
|        | 3          | 25.81                                     | 8.9                                |
| 7      | 1          | 5.42                                      | 8.4                                |
|        | 2          | 4.53                                      | 24.3                               |
|        | 3          | 4.98                                      | 16.1                               |

### 13.2.2 Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 7 serum samples) containing different concentrations of rat IL-17A. 2 standard curves were run on each plate. Data below show the mean rat IL-17A concentration and the coefficient of variation calculated on 18 determinations of each sample (see Table 4). The calculated overall inter-assay coefficient of variation was 7.6%.

Table 4

The mean rat IL-17A concentration and the coefficient of variation of each sample

| Sample | Mean rat IL-17A Concentration ( pg/ml) | Coefficient of Variation (%) |
|--------|--|------------------------------|
| 1      | 75.50                                  | 6.4                          |
| 2      | 43.45                                  | 10.2                         |
| 3      | 20.41                                  | 6.7                          |
| 4      | 12.23                                  | 11.0                         |
| 5      | 75.05                                  | 7.6                          |
| 6      | 25.19                                  | 2.4                          |
| 7      | 4.98                                   | 9.0                          |

### 13.3 Spike Recovery

The spike recovery was evaluated by spiking 3 levels of rat IL-17A into serum, plasma (EDTA, citrate, heparin) and cell culture supernatant samples. Recoveries were determined with 4 replicates each. For recovery data see Table 5.

The unspiked serum, plasma, cell culture supernatant was used as blank in these experiments.

Recoveries were shown to depend on the serum used.

Table 5

| Sample matrix            | Spike high (%) | Spike medium (%) | Spike low (%) |
|--------------------------|----------------|------------------|---------------|
| Serum                    | 44             | 34               | 39            |
| Plasma (EDTA)            | 31             | 20               | 26            |
| Plasma (citrate)         | 59             | 37               | 29            |
| Plasma (heparin)         | 64             | 45               | 37            |
| Cell culture supernatant | 112            | 92               | 103           |

### 13.4 Dilution Parallelism

Serum, plasma cell culture supernatant samples with different levels of rat IL-17A were analysed at serial 2 fold dilutions with 4 replicates each. For recovery data see Table 6.

Table 6

| Sample matrix            | Recovery of Exp. Val. |          |
|--------------------------|-----------------------|----------|
|                          | Range (%)             | Mean (%) |
| Serum                    | 85 - 122              | 102      |
| Plasma (EDTA)            | 93 - 125              | 107      |
| Plasma (citrate)         | 95 - 114              | 106      |
| Plasma (heparin)         | 64 - 126              | 97       |
| Cell culture supernatant | 79 - 89               | 86       |

## **13.5 Sample Stability**

### **13.5.1 Freeze-Thaw Stability**

Aliquots of spiked serum samples were stored at -20°C and thawed 5 times and the rat IL-17A levels determined. There was no significant loss of rat IL-17A immunoreactivity detected by freezing and thawing.

### **13.5.2 Storage Stability**

Aliquots of spiked serum samples were stored at -20°C, 2-8°C room temperature (RT) and at 37°C, and the rat IL-17A level determined after 24 h. There was no significant loss of rat IL-17A immunoreactivity detected during storage at -20°C, 2-8°.

A significant loss of rat IL-17A immunoreactivity was detected during storage at RT and at 37°C after 24 h.

## **13.6 Specificity**

Crossreactivity and interference of circulating factors of the immune system were evaluated by spiking these proteins at physiologically relevant concentrations into a rat IL-17A positive sample.

There was no crossreactivity detected, notably not with rat IFN- $\gamma$ , rat TNF- $\alpha$ , rat IL-1a, rat IL-4, rat MCP-1, rat GM-CSF.

## **13.7 Expected Values**

There were no detectable rat IL-17A levels found.

Elevated rat IL-17A levels depend on the type of immunological disorder.

## 14 Ordering Information

### North America

#### Technical Support:

Research Products:  
888.810.6168  
858.642.2058  
tech@eBioscience.com

Clinical Products:  
877.726.8559  
858.642.2058  
tech@eBioscience.com

#### Customer Service:

888.999.1371  
858.642.2058  
info@eBioscience.com

#### Fax:

858.642.2046

### Europe/International\*

#### Technical Support:

+43 1 796 40 40-120  
tech@eBioscience.com

#### Customer Service:

+43 1 796 40 40-304  
info@eBioscience.com

#### Fax:

+43 1 796 40 40-400



Bender MedSystems GmbH  
Campus Vienna Biocenter 2  
1030 Vienna, Austria  
www.eBioscience.com

\* Customers outside North America and Europe may contact their eBioscience distributor listed on our website at [www.eBioscience.com/distributors](http://www.eBioscience.com/distributors).

## 15 Reagent Preparation Summary

### 15.1 Wash Buffer (1x)

Add **Wash Buffer Concentrate** 20x (50 ml) to 950 ml distilled water.

| Number of Strips | Wash Buffer Concentrate (ml) | Distilled Water (ml) |
|------------------|------------------------------|----------------------|
| 1 - 6            | 25                           | 475                  |
| 1 - 12           | 50                           | 950                  |

### 15.2 Assay Buffer (1x)

Add **Assay Buffer Concentrate** 20x (5 ml) to 95 ml distilled water.

| Number of Strips | Assay Buffer Concentrate (ml) | Distilled Water (ml) |
|------------------|-------------------------------|----------------------|
| 1 - 6            | 2.5                           | 47.5                 |
| 1 - 12           | 5.0                           | 95.0                 |

### 15.3 Biotin-Conjugate

Make a 1:100 dilution of **Biotin-Conjugate** in Assay Buffer (1x):

| Number of Strips | Biotin-Conjugate (ml) | Assay Buffer (1x) (ml) |
|------------------|-----------------------|------------------------|
| 1 - 6            | 0.03                  | 2.97                   |
| 1 - 12           | 0.06                  | 5.94                   |

### 15.4 Streptavidin-HRP

Make a 1:200 dilution of **Streptavidin-HRP** in Assay Buffer (1x):

| Number of Strips | Streptavidin-HRP (ml) | Assay Buffer (1x) (ml) |
|------------------|-----------------------|------------------------|
| 1 - 6            | 0.03                  | 5.97                   |
| 1 - 12           | 0.06                  | 11.94                  |



### **15.5 Rat IL-17A Standard**

Reconstitute lyophilized **rat IL-17A standard** with distilled water.  
(Reconstitution volume is stated on the label of the standard vial.)

## 16 Test Protocol Summary

1. Determine the number of microwell strips required.
2. Wash microwell strips twice with Wash Buffer.
3. Standard dilution on the microwell plate: Add 100 µl Sample Diluent, in duplicate, to all standard wells Pipette 100 µl prepared standard into the first wells and create standard dilutions by transferring 100 µl from well to well. Discard 100 µl from the last wells.  
Alternatively external standard dilution in tubes (see 9.5.1): Pipette 100 µl of these standard dilutions in the microwell strips.
4. Add 100 µl Sample Diluent, in duplicate, to the blank wells.
5. Add 50 µl Sample Diluent to sample wells.
6. Add 50 µl sample in duplicate, to designated sample wells.
7. Prepare Biotin-Conjugate.
8. Add 50 µl Biotin-Conjugate to all wells.
9. Cover microwell strips and incubate 2 hours at room temperature (18° to 25°C).
10. Prepare Streptavidin-HRP.
11. Empty and wash microwell strips 4 times with Wash Buffer.
12. Add 100 µl diluted Streptavidin-HRP to all wells.
13. Cover microwell strips and incubate 1 hour at room temperature.
14. Empty and wash microwell strips 4 times with Wash Buffer.
15. Add 100 µl of TMB Substrate Solution to all wells.
16. Incubate the microwell strips for 30 minutes at room temperature (18° to 25°C).
17. Add 100 µl Stop Solution to all wells.
18. Blank microwell reader and measure colour intensity at 450 nm.

**Note: If instructions in this protocol have been followed samples have been diluted 1: 2 (50 µl sample + 50 µl Sample Diluent), the concentration read from the standard curve must be multiplied by the dilution factor (x 2).**