



BD Cytometric Bead Array (CBA) Mouse Inflammation Kit Instruction Manual



Copyrights

© 2012, Becton, Dickinson and Company. All rights reserved. No part of this publication may be reproduced, transmitted, transcribed, stored in retrieval systems, or translated into any language or computer language, in any form or by any means: electronic, mechanical, magnetic, optical, chemical, manual, or otherwise, without prior written permission from BD Biosciences.

The information in this guide is subject to change without notice. BD Biosciences reserves the right to change its products and services at any time to incorporate the latest technological developments. Although this guide has been prepared with every precaution to ensure accuracy, BD Biosciences assumes no liability for any errors or omissions, nor for any damages resulting from the application or use of this information. BD Biosciences welcomes customer input on corrections and suggestions for improvement.

Trademarks

FCAP Array is a trademark of Soft Flow Hungary Ltd.

Mac is a trademark of Apple Computer, Inc., registered in the US and other countries.

BD, BD Logo and all other trademarks are property of Becton, Dickinson and Company.
© 2012 BD

Regulatory information

BD flow cytometers are Class 1 Laser Products.

For Research Use Only. Not for use in diagnostic or therapeutic procedures.

History

Revision	Date	Change made
23-12720-00 Rev. 01	1/2011	New document
23-12720-01 Rev. 01	2/2012	Updated image

Contents

Chapter 1: About this kit	5
Purpose of this kit	6
Limitations	8
Kit contents	9
Storage and handling	11
Chapter 2: Before you begin	13
Workflow overview	14
Required materials	15
Chapter 3: Assay preparation	17
Preparing Mouse Inflammation Standards	18
Mixing Mouse Inflammation Capture Beads	20
Diluting samples	21
Chapter 4: Assay procedure	23
Performing the Mouse Inflammation Assay	24
Data analysis	27
Chapter 5: Performance	29
Theoretical limit of detection	30
Recovery	31
Linearity	32
Specificity	33
Precision	35
Chapter 6: Reference	37
Troubleshooting	38
References	40

About this kit

This section covers the following topics:

- [Purpose of this kit \(page 6\)](#)
- [Limitations \(page 8\)](#)
- [Kit contents \(page 9\)](#)
- [Storage and handling \(page 11\)](#)

Purpose of this kit

Use of the kit The BD™ CBA Mouse Inflammation Kit can be used to quantitatively measure Interleukin-6 (IL-6), Interleukin-10 (IL-10), Monocyte Chemoattractant Protein-1 (MCP-1), Interferon- γ (IFN- γ), Tumor Necrosis Factor (TNF), and Interleukin-12p70 (IL-12p70) protein levels in a single sample. The kit performance has been optimized for analysis of specific proteins in tissue culture supernatants, EDTA plasma, and serum samples. The kit provides sufficient reagents for 80 tests.

Principle of CBA assays BD CBA assays provide a method of capturing a soluble analyte or set of analytes with beads of known size and fluorescence, making it possible to detect analytes using flow cytometry.

Each capture bead in the kit has been conjugated with a specific antibody. The detection reagent provided in the kit is a mixture of phycoerythrin (PE)-conjugated antibodies, which provides a fluorescent signal in proportion to the amount of bound analyte.

When the capture beads and detector reagent are incubated with an unknown sample containing recognized analytes, sandwich complexes (capture bead + analyte + detection reagent) are formed. These complexes can be measured using flow cytometry to identify particles with fluorescence characteristics of both the bead and the detector.

Principle of the test

Six bead populations with distinct fluorescence intensities have been coated with capture antibodies specific for IL-6, IL-10, MCP-1, IFN- γ , TNF, and IL-12p70 proteins. The six bead populations are mixed together to form the bead array, which is resolved in a red channel of a flow cytometer (see Figure 1).

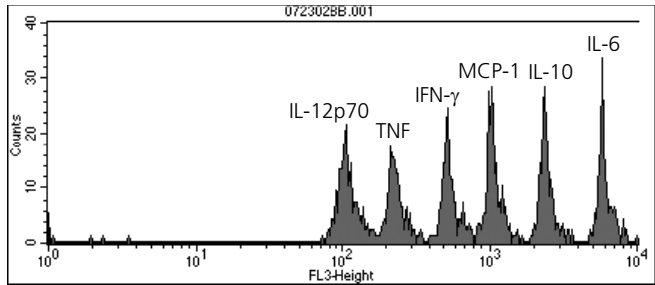


Figure 1

During the assay procedure, you will mix the chemokine capture beads with the recombinant standards or unknown samples and incubate them with the PE-conjugated detection antibodies to form sandwich complexes. The intensity of PE fluorescence of each sandwich complex reveals the concentration of that cytokine. After acquiring samples on a flow cytometer, use FCAP Array™ software to generate results in graphical and tabular format.

Advantages over ELISA

The broad dynamic range of fluorescence detection via flow cytometry and the efficient capturing of analytes via suspended particles enable BD CBA assays to measure the concentration of an unknown in substantially less time and using fewer sample dilutions compared to conventional ELISA methodology.

- The required sample volume is approximately one-sixth the quantity necessary for conventional ELISA assays due to the detection of six analytes in a single sample.
 - A single set of diluted standards is used to generate a standard curve for each analyte.
 - A BD CBA experiment takes less time than a single ELISA and provides results that would normally require six conventional ELISAs.
-

Limitations

Assay limitations The theoretical limit of detection of the BD CBA Mouse Inflammation Kit is comparable to conventional ELISA, but due to the complexity and kinetics of this multi-analyte assay, the actual limit of detection in a given experiment may vary slightly. Note the reduced sensitivity of the Mouse MCP-1 assay. See [Theoretical limit of detection \(page 30\)](#) and [Precision \(page 35\)](#).

The BD CBA assay is not recommended for use on stream-in-air instruments for which signal intensities may be reduced, adversely affecting assay sensitivity. Stream-in-air instruments include the BD FACStar™ Plus, BD FACSVantage™, and BD Influx™ flow cytometers (BD Biosciences).

Serum spike recoveries for IL-10 and TNF are lower than for the other proteins in this assay. This variation is due to assay conditions and serum proteins. It may affect quantitation of these proteins in serum samples.

Quantitative results or protein levels for the same sample or recombinant protein run in ELISA and BD CBA assays may differ. A spike recovery assay can be performed using an ELISA standard followed by BD CBA analysis to assess possible differences in quantitation.

This kit is designed to be used as an integral unit Do not mix components from different batches or kits.

Kit contents

Contents This kit contains the following components sufficient for 80 tests.

Vial label	Reagent	Quantity
A1	Mouse IL-6 Capture Beads	1 vial, 0.8 mL
A2	Mouse IL-10 Capture Beads	1 vial, 0.8 mL
A3	Mouse MCP-1 Capture Beads:	1 vial, 0.8 mL
A4	Mouse IFN- γ Capture Beads	1 vial, 0.8 mL
A5	Mouse TNF Capture Beads	1 vial, 0.8 mL
A6	Mouse IL-12p70 Capture Beads	1 vial, 0.8 mL
B	Mouse Inflammation PE Detection Reagent	1 vial, 4 mL
C	Mouse Inflammation Standards	2 vials, 0.2 mL lyophilized
D	Cytometer Setup Beads	1 vial, 1.5 mL

Vial label	Reagent	Quantity
E1	PE Positive Control Detector	1 vial, 0.5 mL
E2	FITC Positive Control Detector	1 vial, 0.5 mL
F	Wash Buffer	1 bottle, 130 mL
G	Assay Diluent	1 bottle, 30 mL

Bead reagents

Mouse Inflammation Capture Beads (A1–A6): An 80-test vial of each specific capture bead (A1–A6). The specific capture beads, having discrete fluorescence intensity characteristics, are distributed from brightest (A1) to dimmest (A6).

Cytometer Setup Beads (D): A 30-test vial of setup beads for setting the initial instrument PMT voltages and compensation settings is sufficient for 10 instrument setup procedures. The Cytometer Setup Beads are formulated for use at 50 μ L per test.

Antibody and standard reagents

Mouse Inflammation PE Detection Reagent (B): An 80-test vial of PE-conjugated anti-mouse IL-6, IL-10, MCP-1, IFN- γ , TNF, and IL-12p70 antibodies, formulated for use at 50 μ L per test.

Mouse Inflammation Standards (C): Two vials containing lyophilized recombinant mouse proteins. Each vial should be reconstituted in 2 mL of Assay Diluent to prepare the top standard.

PE Positive Control Detector (E1): A 10-test vial of PE-conjugated antibody control that is formulated for use at 50 μ L per test. This reagent is used with the Cytometer Setup Beads to set the initial instrument compensation settings.

FITC Positive Control Detector (E2): A 10-test vial of FITC-conjugated antibody control that is formulated for use at 50 μL per test. This reagent is used with the Cytometer Setup Beads to set the initial instrument compensation settings.

Buffer reagents

Wash Buffer (F): A 130-mL bottle of phosphate buffered saline (PBS) solution (1X), containing protein and detergent, used for wash steps and to resuspend the washed beads for analysis.

Assay Diluent (G): A 30-mL bottle of a buffered protein solution (1X) used to reconstitute and dilute the Mouse Inflammation Standards and to dilute test samples.

Note: Source of all serum proteins is from USDA inspected abattoirs located in the United States.

Storage and handling

Storage

Store all kit components at 2 to 8°C. Do not freeze.

Warning

Components A1–A6, B, D, E1, E2, F, and G contain sodium azide. Sodium azide yields a highly toxic hydrazoic acid under acidic conditions. Dilute azide compounds in running water before discharging to avoid accumulation of potentially explosive deposits in plumbing.

2

Before you begin

This section covers the following topics:

- [Workflow overview \(page 14\)](#)
- [Required materials \(page 15\)](#)

Workflow overview

Workflow

The overall workflow consists of the following steps.

Step	Description
1	Preparing Mouse Inflammation Standards (page 18)
2	Mixing Mouse Inflammation Capture Beads (page 20)
3	Diluting samples (page 21)
4	Performing instrument setup with Cytometer Setup Beads (instructions can be found at bdbiosciences.com/cbasetup) Can be performed during the incubation in step 5 .
5	Performing the Mouse Inflammation Assay (page 24)
6	Acquiring samples (instructions can be found at bdbiosciences.com/cbasetup)
7	Data analysis (page 27)

Incubation times

To help you plan your work, the incubation times are listed in the following table.

Procedure	Incubation time
Preparing standards	15 minutes
Preparing Cytometer Setup Beads	30 minutes
Performing the assay	2 hours

Required materials

Materials required but not provided

In addition to the reagents provided in the BD CBA Mouse Inflammation Kit, the following items are also required:

- A dual-laser flow cytometer equipped with a 488-nm or 532-nm and a 633-nm or 635-nm laser capable of distinguishing 576-nm, 660-nm, and >680-nm fluorescence. The following table lists examples of compatible instrument platforms.

Flow cytometer	Reporter channel	Bead channels
BD FACSAArray™	Yellow	Red
BD FACSCanto™ platform BD™ LSR platform BD FACSAria™ platform	PE	APC
BD FACSCalibur™ (single laser) BD FACSCalibur (dual laser)	FL2	FL3 FL4
Note: Visit bdbiosciences.com/cbasetup for setup protocols.		

- BD Falcon™ 12 × 75-mm sample acquisition tubes for a flow cytometer (Catalog No. 352008)
- 15-mL conical, polypropylene tubes (BD Falcon, Catalog No. 352097), or equivalent

Note: FCAP Array software (Catalog No. 641488 [PC] or 645447 [Mac®])

**Materials
required for
plate loader-
equipped flow
cytometers**

- Millipore MultiScreen_{HTS}-BV 1.2- μ m Clear non-sterile filter plates [Catalog No. MSBVN1210 (10 pack) or MSBVN1250 (50 pack)]
 - Millipore MultiScreen_{HTS} Vacuum Manifold (Catalog No. MSVMHTS00)
 - MTS 2/4 Digital Stirrer, IKA Works, VWR (Catalog No. 82006-096)
 - Vacuum source
 - Vacuum gauge and regulator (if not using the recommended manifold)
-

3

Assay preparation

This section covers the following topics:

- [Preparing Mouse Inflammation Standards \(page 18\)](#)
- [Mixing Mouse Inflammation Capture Beads \(page 20\)](#)
- [Diluting samples \(page 21\)](#)

Preparing Mouse Inflammation Standards

Purpose of this procedure

The Mouse Inflammation Standards are lyophilized and should be reconstituted and serially diluted immediately before mixing with the Capture Beads and the PE Detection Reagent.


You must prepare fresh cytokine standards to run with each experiment. Do not store or reuse reconstituted or diluted standards.

Procedure

To reconstitute and serially dilute the standards:

1. Open one vial of lyophilized Mouse Inflammation Standards. Transfer the standard spheres to a 15-mL conical, polypropylene tube. Label the tube “Top Standard.”
2. Reconstitute the standards with 2.0 mL of Assay Diluent.
 - a. Allow the reconstituted standard to equilibrate for at least 15 minutes at room temperature.
 - b. Gently mix the reconstituted protein by pipet only. Do not vortex or mix vigorously.
3. Label eight 12 x 75-mm tubes and arrange them in the following order: 1:2, 1:4, 1:8, 1:16, 1:32, 1:64, 1:128, and 1:256.
4. Pipette 300 μ L of Assay Diluent into each of the remaining tubes.
5. Perform a serial dilution:
 - a. Transfer 300 μ L from the Top Standard to the 1:2 dilution tube and mix thoroughly by pipet only. Do not vortex.

- b. Continue making serial dilutions by transferring 300 μL from the 1:2 tube to the 1:4 tube and so on to the 1:256 tube.
- c. Mix thoroughly by pipet only. Do not vortex.

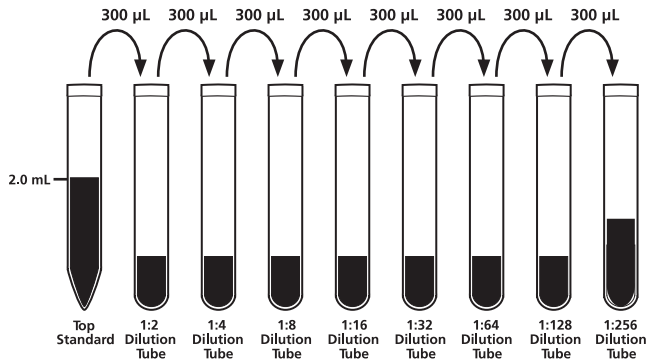

6. Prepare one 12 x 75-mm tube containing Assay Diluent to serve as the 0-pg/mL negative control.

Concentration of standards See [Performing the Mouse Inflammation Assay \(page 24\)](#) for a list of the concentration (pg/mL) of all six recombinant proteins in each standard dilution.

Next step Proceed to [Mixing Mouse Inflammation Capture Beads \(page 20\)](#).

Mixing Mouse Inflammation Capture Beads

Purpose of this procedure The Capture Beads are bottled individually (A1–A6). You must pool all six bead reagents immediately before using them in the assay.

Procedure **To mix the Capture Beads:**

1. Determine the number of assay tubes (including standards and controls) that are required for the experiment (for example, 8 unknowns + 9 standard dilutions + 1 negative control = 18 assay tubes).
2. Vigorously vortex each Capture Bead suspension for 3 to 5 seconds before mixing.

Note: The antibody-conjugated beads will settle out of suspension over time. Vortex the vial immediately before taking a bead-suspension aliquot.
3. Add a 10- μ L aliquot of each Capture Bead, for each assay tube to be analyzed, into a single tube labeled “Mixed Capture Beads” (for example, 10 μ L of IL-6 Capture Beads \times 18 assay tubes = 180 μ L of IL-6 Capture Beads required).
4. Vortex the bead mixture thoroughly.

Next step The mixed Capture Beads are now ready to be transferred to the assay tubes. Discard excess mixed Capture Beads. Do not store after mixing.

To begin the assay, proceed to [Performing the Mouse Inflammation Assay \(page 24\)](#). If you need to dilute samples having high-protein concentration, proceed to [Diluting samples \(page 21\)](#).

Diluting samples

Purpose of this procedure The standard curve for each protein covers a defined set of concentrations from 20 to 5,000 pg/mL. It might be necessary to dilute test samples to ensure that their median fluorescence values fall within the range of the generated standard curve. For best results, dilute samples that are known or assumed to contain high levels of a given protein.

Procedure To dilute samples with a known high-protein concentration:

1. Dilute the sample by the desired dilution factor (ie, 1:2, 1:10, or 1:100) using the appropriate volume of Assay Diluent.
2. Mix sample dilutions thoroughly.

Next step Perform instrument setup using the Cytometer Setup Beads. For details, go to bdbiosciences.com/cbasetup and select the appropriate flow cytometer under CBA Kits: Instrument Setup.

Of, if you wish to begin staining your samples for the assay, proceed to [Performing the Mouse Inflammation Assay \(page 24\)](#), and you can perform instrument setup during the 2-hour staining incubation.

4

Assay procedure

This section covers the following topics:

- [Performing the Mouse Inflammation Assay \(page 24\)](#)
- [Data analysis \(page 27\)](#)

Performing the Mouse Inflammation Assay

Purpose of this procedure

- Prepare the standards as described in [Preparing Mouse Inflammation Standards \(page 18\)](#).
- Mix the Capture Beads as described in [Mixing Mouse Inflammation Capture Beads \(page 20\)](#).
- If necessary, dilute the unknown samples. See [Diluting samples \(page 21\)](#)

Procedure for tubes

To perform the assay:

1. Vortex the mixed Capture Beads and add 50 μ L to the all assay tubes.
2. Add 50 μ L of the Mouse Inflammation Standard dilutions to the control assay tubes as listed in the following table.

Tube label	Concentration (pg/mL)	Standard dilution
1	0 (negative control)	no standard dilution (Assay Diluent only)
2	20	1:256
3	40	1:128
4	80	1:64
5	156	1:32
6	312	1:16
7	625	1:8
8	1,250	1:4
9	2,500	1:2
10	5,000	Top Standard

3. Add 50 μ L of each unknown sample to the appropriately labeled sample assay tubes.

4. Add 50 μL of the Mouse Inflammation PE Detection Reagent to all assay tubes.
 5. Incubate the assay tubes for 2 hours at room temperature, protected from light.
Note: If you have not yet performed cytometer setup, you may wish to do so during this incubation.
 6. Add 1 mL of Wash Buffer to each assay tube and centrifuge at 200g for 5 minutes.
 7. Carefully aspirate and discard the supernatant from each assay tube.
 8. Add 300 μL of Wash Buffer to each assay tube to resuspend the bead pellet.
-

Procedure for filter plates

To perform the assay:

1. Wet the plate by adding 100 μL of wash buffer to each well.
2. Place the plate on the vacuum manifold.
3. Aspirate for 2 to 10 seconds until the wells are drained.
4. Remove the plate from the manifold, then blot the bottom of the plate on paper towels.
5. Add 50 μL of each of the following to the wells in the filter plate:
 - Capture Beads (vortex before adding)
 - Standard or sample (add standards from the lowest concentration to the highest, followed by samples)
 - Mouse Inflammation PE Detection Reagent
6. Cover the plate and shake it for 5 minutes at 1,100 rpm on a plate shaker.

7. Incubate the plate for 2 hours at room temperature on a non-absorbent, dry surface.
Note: Place the plate on a non-absorbent, dry surface during incubation. Absorbent or wet surfaces can cause the contents of the wells to leak.
8. Remove the cover from the plate and apply the plate to the vacuum manifold.
9. Vacuum aspirate for 2 to 10 seconds until the wells are drained.
10. Remove the plate from the manifold, then blot the bottom of the plate on paper towels after aspiration.
11. Add 120 μ L of wash buffer to each well to resuspend the beads.
12. Cover the plate and shake it for 2 minutes at 1,100 rpm before you begin sample acquisition.

Next step

Acquire the samples on the flow cytometer. For details, go to bdbiosciences.com/cbasetup and select the appropriate flow cytometer under CBA Kits: Instrument Setup.

CBA samples must be acquired on the same day they are prepared. Prolonged storage of samples, once the assay is complete, can lead to increased background and reduced sensitivity.

To facilitate the analysis of samples using the FCAP Array software, we recommend the following guidelines:

- Acquire standards from lowest (0 pg/mL) to highest (Top Standard) concentration, followed by the test samples.
- If running sample dilutions, acquire sequentially starting with the most concentrated sample.


- Store all FCS files (standards and samples) in a single folder.

When you are finished acquiring samples, proceed to [Data analysis \(page 27\)](#).


Data analysis

How to analyze Analyze BD CBA Mouse Inflammation Kit data using FCAP Array software. For instructions on analysis, go to bdbiosciences.com/cbasetup and see the *Guide to Analyzing Data from BD CBA Kits Using FCAP Array Software*.


Typical data The following data, acquired using BD CellQuest™ software, shows standards and detectors alone.




Negative control



Standards 80 pg/mL









Standards 625 pg/mL



Standards 5000 pg/mL

Standard curve examples

The following graphs represent standard curves from the BD CBA Mouse Inflammation Standards.

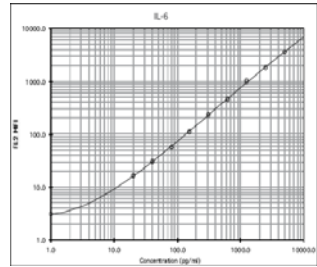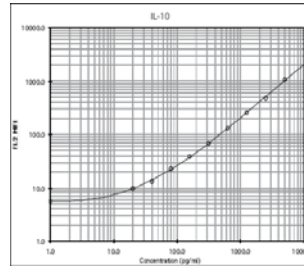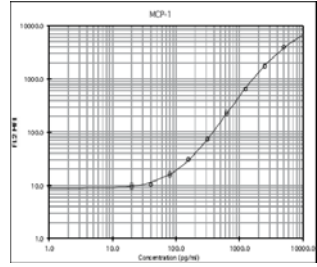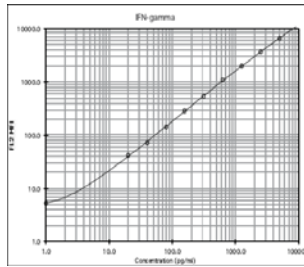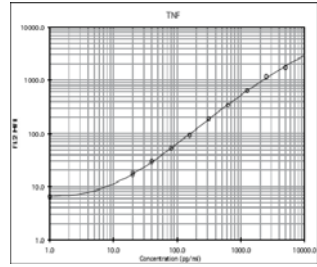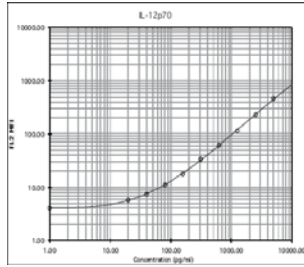

5

Performance

This section covers the following topics:

- [Theoretical limit of detection \(page 30\)](#)
- [Recovery \(page 31\)](#)
- [Linearity \(page 32\)](#)
- [Specificity \(page 33\)](#)
- [Precision \(page 35\)](#)

Theoretical limit of detection

Experiment details

The individual standard curve range for a given protein defines the minimum and maximum quantifiable levels using the BD CBA Mouse Inflammation Kit (ie, 20 pg/mL and 5,000 pg/mL). By applying the 4-parameter curve fit option, it is possible to extrapolate values for sample intensities not falling within the limits of the standard curve. It is up to the researcher to decide the best method for calculating values for unknown samples using this assay. The theoretical limit of detection for each protein using the BD CBA Mouse Inflammation Kit is defined as the corresponding concentration at two standard deviations above the median fluorescence of 20 replicates of the negative control (0 pg/mL).

Limit of detection data

Cytokine	Median fluorescence	Standard deviation	Limit of detection (pg/mL)
IL-6	3.3	0.3	5
IL-10	5.9	0.5	17.5
MCP-1	9.3	0.4	52.7
IFN- γ	5.4	0.4	2.5
TNF	6.5	0.3	7.3
IL-12p70	4.1	0.4	10.7

Recovery

Experiment details

Individual protein was spiked into various matrices at three different levels within the assay range. The cell culture media used in these experiments were not diluted before addition of the protein. The pooled mouse serum samples in these experiments were diluted 1:4 in Assay Diluent before addition of the cytokine protein. Results are compared with the same concentrations of the proteins spiked in the Assay Diluent.

Recovery data

Protein	Matrix	Standard spike conc. (pg/mL)	Observed in given matrix (pg/mL)	% Recovery
IL-6	Pooled mouse sera (1:4 dilution)	2,500	1,990.3	80%
		625	458.4	73%
		80	62.3	78%
	Cell culture media	2,500	2,476.7	99%
		625	594.3	95%
		80	95.8	120%
IL-10	Pooled mouse sera (1:4 dilution)	2,500	918.5	37%
		625	208.2	33%
		80	11.2	14%
	Cell culture media	2,500	2,326.7	93%
		625	581.9	93%
		80	99.7	125%
MCP-1	Pooled mouse sera (1:4 dilution)	2,500	1,954.5	78%
		625	448.5	72%
		80	35.8	45%
	Cell culture media	2,500	2,474.2	99%
		625	579.2	93%
		80	82.7	103%

Protein	Matrix	Standard spike conc. (pg/mL)	Observed in given matrix (pg/mL)	% Recovery
IFN- γ	Pooled mouse sera (1:4 dilution)	2,500	1,386.8	55%
		625	323.9	52%
		80	46.6	58%
	Cell culture media	2,500	2,423.9	97%
		625	584.8	94%
		80	79.7	100%
TNF	Pooled mouse sera (1:4 dilution)	2,500	779.8	31%
		625	181.0	29%
		80	26.8	34%
	Cell culture media	2,500	2,651.7	106%
		625	587.5	94%
		80	83.3	104%
IL-12p70	Pooled mouse sera (1:4 dilution)	2,500	1,468.5	59%
		625	350.5	56%
		80	23.5	29%
	Cell culture media	2,500	2,349.0	94%
		625	538.2	86%
		80	73.9	92%

Linearity

Experiment details

In two experiments, the following matrices were spiked with IL-6, IL-10, MCP-1, IFN- γ , TNF, and IL-12p70 and were then serially diluted with Assay Diluent.

Linearity data

Matrix	Dilution	Observed (pg/mL)					
		IL-6	IL-10	MCP-1	IFN- γ	TNF	IL-12p70
Pooled mouse sera (1:4 starting dilution)	1:4	4,041.8	1,935.9	4,052.3	2,877.2	1,601.9	3,372.1
	1:8	2,128.9	1,244.7	2,227.9	1,588.3	1,001.2	1,675.3
	1:16	1,086.9	797.3	1,183.0	958.8	630.0	913.5
	1:32	529.3	438.6	619.2	520.4	370.7	491.7
	1:64	277.1	238.7	291.8	255.4	211.5	242.8
	1:128	136.9	136.7	160.5	140.1	122.0	142.2
	1:256	70.6	76.7	77.8	69.9	73.4	82.7
	1:512	33.2	29.9	22.3	34.2	38.0	34.4
	1:1,024	14.5	14.2	0.0	18.1	17.5	12.9
	Slope	1.006	0.882	1.029	0.922	0.801	0.961
Cell culture media	Neat	4,347.7	4,870.6	4,946.1	4,518.4	4,407.9	4,615.7
	1:2	2,370.3	2,373.0	2,379.3	2,392.4	2,576.8	2,426.8
	1:4	1,207.6	1,271.9	1,202.2	1,255.9	1,330.1	1,203.6
	1:8	572.5	588.9	593.1	640.7	616.1	588.7
	1:16	295.0	312.8	296.4	303.3	321.2	328.2
	1:32	132.3	151.0	135.7	145.3	146.3	130.6
	1:64	68.9	72.9	57.8	72.2	75.8	63.0
	1:128	39.8	44.2	34.6	38.6	43.2	44.5
	1:256	17.5	21.6	18.1	20.9	21.6	19.1
	Slope	0.998	0.979	1.026	0.999	0.979	1.113


Specificity

Experiment details


The antibody pairs used in the BD CBA Mouse Inflammation assay have been screened for specific reactivity with their specific proteins. Analysis of samples containing only a single recombinant protein found no cross-reactivity or background detection of protein in other Capture Bead populations using this assay.

Specificity data


The following plots show BD CellQuest data for the detection of individual proteins.




Mouse IL-6




Mouse IL-10




Mouse MCP-1



Mouse IFN- γ



Mouse TNF



Mouse IL-12p70

Precision

Intra-assay precision

Ten replicates of each of three different levels of IL-6, IL-10, MCP-1, IFN- γ , TNF, and IL-12p70 were tested.

Protein	Actual mean conc. (pg/mL)	SD	%CV
IL-6	76	4	5%
	551	20	4%
	2,107	94	5%
IL-10	78	7	9%
	573	19	3%
	1,987	104	5%
MCP-1	66	6	10%
	614	9	2%
	2,300	46	2%
IFN- γ	73	3	4%
	633	19	3%
	2,239	103	5%
TNF	69	2	3%
	597	21	4%
	2,358	103	4%
IL-12p70	66	10	15%
	600	23	4%
	2,238	103	5%

**Inter-assay
precision**

Inter-assay: Three different levels of IL-6, IL-10, MCP-1, IFN- γ , TNF, and IL-12p70 (80, 625, and 2,500 pg/mL) were tested in four experiments.

Note: Eight replicates (total number of assay tubes) were tested for each concentration of protein.

Protein	Actual mean conc. (pg/mL)	SD	% CV
IL-6	79	8	10%
	557	62	11%
	2,426	198	8%
IL-10	71	10	14%
	581	45	8%
	2,329	162	7%
MCP-1	58	11	19%
	598	33	5%
	2,431	51	2%
IFN- γ	75	6	8%
	631	40	6%
	2,425	120	5%
TNF	75	8	11%
	592	40	7%
	2,697	155	6%
IL-12p70	72	7	9%
	590	30	5%
	2,430	70	3%

6

Reference

This section covers the following topics:

- [Troubleshooting \(page 38\)](#)
- [References \(page 40\)](#)

Troubleshooting

Recommended actions

These are the actions we recommend taking if you encounter the following problems.

Note: For best performance, vortex samples immediately before analyzing on a flow cytometer.

Note: The BD CBA Mouse Inflammation assay has been shown to detect TNF produced by the activation of cells from the rat model. Direct quantitation of proteins from the rat model has not been validated using this kit and results may vary.

Problem	Recommended action
Variation between duplicate samples	Vortex Capture Beads before pipetting. Beads can aggregate.
Low bead number in samples	<ul style="list-style-type: none"> ● Avoid aspiration of beads during wash step. ● Do not wash or resuspend beads in volumes higher than recommended volumes.
High background	<ul style="list-style-type: none"> ● Test various sample dilutions. The sample may be too concentrated. ● Remove excess Mouse Inflammation PE Detection Reagent by increasing the number of wash steps, since the background may be due to non-specific binding.
Little or no detection of protein in sample	Sample may be too dilute. Try various sample dilutions.
Less than six bead populations are observed during analysis, or distribution is unequal	<ul style="list-style-type: none"> ● Ensure that equal volumes of beads were added to each assay tube. ● Vortex Capture Bead vials before taking aliquots. Once Capture Beads are mixed, vortex to ensure that the beads are distributed evenly throughout the solution.

Problem	Recommended action
Debris (FSC/SSC) during sample acquisition	<ul style="list-style-type: none"> ● Increase FSC threshold or further dilute samples. ● Increase the number of wash steps, if necessary. ● Make a tighter FSC/SSC region gate around the bead population.
Overlap of bead population fluorescence (FL3) during acquisition	This may occur in samples with very high protein concentration. Ensure that instrument settings have been optimized using the Cytometer Setup Beads.
Standards assay tubes show low fluorescence or poor standard curve	<p>Ensure that all components are properly prepared and stored.</p> <p>Use a new vial of standard with each experiment, and once reconstituted, do not use after 12 hours.</p> <p>Ensure that incubation times were appropriate.</p>
All samples are positive or above the high standard median fluorescence value	Dilute the samples further. The samples may be too concentrated.
Biohazardous samples	It is possible to treat samples briefly with 1% paraformaldehyde before analyzing on the flow cytometer. However, this may affect assay performance and should be validated.

References

Related publications

1. Bishop JE, Davis KA. A flow cytometric immunoassay for β 2-microglobulin in whole blood. *J Immunol Methods*. 1997;210:79–87.
2. Camilla C, Defoort JP, Delaage M, et al. A new flow cytometry-based multi-assay system. 1. Application to cytokine immunoassays. *Cytometry Suppl*. 1998;8:132.
3. Carson R, Vignali D. Simultaneous quantitation of 15 cytokines using a multiplexed flow cytometric assay. *J Immunol Methods*. 1999;227:41–52.
4. Chen R, Lowe L, Wilson JD, et al. Simultaneous quantification of six human cytokines in a single sample using microparticle-based flow cytometric technology. *Clin Chem*. 1999;45:1693–1694.
5. Collins DP, Luebering BJ, Shaut DM. T-lymphocyte functionality assessed by analysis of cytokine receptor expression, intracellular cytokine expression, and femtomolar detection of cytokine secretion by quantitative flow cytometry. *Cytometry*. 1998;33:249–255.
6. Fulton RJ, McDade RL, Smith PL, Kienker LJ, Kettman JR Jr. Advanced multiplexed analysis with the FlowMetrix system. *Clin Chem*. 1997;43:1749–1756.
7. Kricka LJ. Simultaneous multianalyte immunoassays. In: Diamandis EP, Christopoulos TK, eds. *Immunoassay*. Academic Press. 1996:389–404.

8. Lund-Johansen F, Davis K, Bishop J, de Waal Malefyt R. Flow cytometric analysis of immunoprecipitates: high-throughput analysis of protein phosphorylation and protein-protein interactions. *Cytometry*. 2000;39:250–259.
 9. McHugh TM. Flow microsphere immunoassay for the quantitative and simultaneous detection of multiple soluble analytes. *Methods Cell Biol*. 1994;42:575–595.
 10. Oliver KG, Kettman JR, Fulton RJ. Multiplexed analysis of human cytokines by use of the FlowMetrix system. *Clin Chem*. 1998;44:2057–2060.
 11. Stall A, Sun Q, Varro R, et al. A single tube flow cytometric multibead assay for isotyping mouse monoclonal antibodies. Abstract LB77. Experimental Biology Meeting 1998 (late-breaking abstracts).
 12. Cook EB, Stahl JL, Lowe L, et al. Simultaneous measurement of six cytokines in a single sample of human tears using microparticle-based flow cytometry: allergics vs non-allergics. *J Immunol Methods*. 2001;254:109–118.
 13. Dotti G, Savoldo B, Takahashi S, et al. Adenovector-induced expression of human-CD40-ligand (hCD40L) by multiple myeloma cells: A model for immunotherapy. *Exp Hematol*. 2001;29:952–961.
-

United States

877.232.8995

Canada

800.268.5430

Europe

32.2.400.98.95

Japan

0120.8555.90

Asia/Pacific

65.6861.0633

Latin America/Caribbean

55.11.5185.9995



**Becton, Dickinson and Company
BD Biosciences**

2350 Qume Dr.

San Jose, CA 95131 USA

(US) Ordering 855.236.2772

Technical Service 877.232.8995

Fax 800.325.9637

answers@bd.com

bdbiosciences.com