

## Technical Data Sheet Human IgG2 Flex Set


### Product Information

<b>Material Number:</b>	558676
<b>Size:</b>	100 Tests
<b>Bead Position:</b>	C5
<b>Assay Range:</b>	13.3-3400 ng/mL
<b>Reactivity:</b>	QC Testing: Human

Component Description: Human Ig Standard  
 Component Mat. No: 51-9004553  
 Component Storage Buffer: Lyophilized in an aqueous buffered solution containing BSA and ProClin™ 150.

Component Description: Human IgG2 PE\* Detection Reagent  
 Component Mat. No: 51-9005008  
 Component Storage Buffer: Aqueous buffered solution containing BSA and ≤0.09% sodium azide.

Component Description: Human IgG2 Capture Bead C5  
 Component Mat. No: 51-9005010  
 Component Storage Buffer: Aqueous buffered solution containing BSA and ≤0.09% sodium azide.

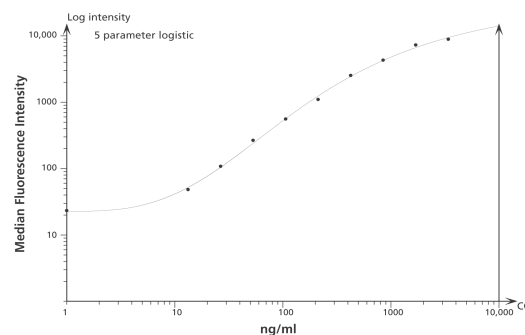

**Figure 1. Example BD CBA Human IgG2 Flex Set standard curve.** Data acquired on a BD FACsArray bioanalyzer and analyzed using the FCAP Array Software (Cat. No. 641488).

### Description

The BD™ CBA Human IgG2 Flex Set is a bead-based immunoassay capable of measuring human immunoglobulin G subclass 2 (IgG2) in serum and plasma samples. Human reactivity was determined by testing samples with the BD CBA Human IgG2 Flex Set. The biology and function of IgG2 has been extensively reviewed in the literature. For more information on bead-based immunoassays, refer to the product insert for the BD CBA Human Immunoglobulin Master Buffer Kit (Cat. No. 558683).

This BD™ CBA Flex Set contains one vial each of Capture Bead and PE Detection Reagent and two vials of Standard. The Capture Bead and PE Detection Reagent components of this flex set have been formulated to a 50x concentration to ensure product performance when multiplexed. The Standard component is lyophilized and when reconstituted in 1.0 ml Assay Diluent has an IgG2 protein concentration of 3,400 ng/ml. Discard unused reconstituted standard, do not store or reuse. Store lyophilized standard and other components at 4°C. Protect PE Detection Reagent from prolonged exposure to light.

### Application Notes

**Recommended Assay Procedure:** The BD CBA Human IgG2 Flex Set must be used in conjunction with a BD CBA Human Immunoglobulin Master Buffer Kit (Cat. No. 558683, 100 tests), a flow cytometer, and the FCAP Array™ Software (Cat. No. 641488). Detailed instructions on the use of this product can be found in the manual for the BD CBA Human Immunoglobulin Master Buffer Kit. When following the directions in the Master Buffer Kit, the top standard point for the BD CBA Human IgG2 Flex Set will be 3,400 ng/ml. An example standard curve is shown in Figure 1. The Human Ig Standard provided in this Flex Set is derived from human serum and contains Human IgG1, IgG2, IgG3, IgG4, IgM, IgA and IgE proteins. Only one Human Ig Standard vial is needed when preparing standard curves for a multiplex assay using multiple Human Immunoglobulin Flex Set assays. The BD CBA Human IgG2 Flex Set cannot be used in the same assay well with the following BD CBA Immunoglobulin Flex Set reagents:

### BD Biosciences

bdbiosciences.com

United States	Canada	Europe	Japan	Asia Pacific	Latin America/Caribbean
877.232.8995	800.268.5430	32.2.400.98.95	0120.8555.90	65.6861.0633	55.11.5185.9995

For country contact information, visit [bdbiosciences.com/contact](http://bdbiosciences.com/contact)

*Conditions: The information disclosed herein is not to be construed as a recommendation to use the above product in violation of any patents. BD Biosciences will not be held responsible for patent infringement or other violations that may occur with the use of our products. Purchase does not include or carry any right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of Becton, Dickinson and Company is strictly prohibited.*

For Research Use Only, Not for use in diagnostic or therapeutic procedures. Not for resale.

Unless otherwise noted, BD, BD Logo and all other trademarks are property of Becton, Dickinson and Company. © 2014 BD



Flex Set	Bead Position	Catalog Number
BD CBA Human IgG1 Flex Set	C4	558675
BD CBA Human Total IgG Flex Set	C6	558679

Due to the levels of immunoglobulin protein in typical samples and specific assay conditions, the BD CBA Human IgG2 Flex Set should not be used in the same assay well with any non-BD CBA Human Immunoglobulin Flex Set reagents (such as BD CBA Mouse Soluble Protein, Human Soluble Protein or Cell Signaling Flex Sets). For an updated assay compatibility chart for the BD CBA Human Immunoglobulin Flex Sets, please refer to the BD CBA Flex Set System homepage at <http://www.bdbiosciences.com/flexset>.

## Performance

**Limit of Detection:** The theoretical limit of detection is 0.85 ng/ml and was determined by evaluating the estimated result of the average MFI of the negative control (0 pg/ml,  $n=30$ ) + 2 standard deviations.

Specificity		Inter-Assay Reproducibility			Intra-Assay Reproducibility		
		Mean (ng/ml)	Standard Deviation	%CV	Mean (ng/ml)	Standard Deviation	%CV
Human IgG2	Sample 1	51.2	3.9	8%	47.3	2.6	6%
	Sample 2	197.9	15.4	8%	176.5	7.9	4%
	Sample 3	837.3	95.2	11%	680.5	31.1	5%

**Reproducibility:** The inter-assay and intra-assay reproducibility were determined for the BD CBA Human IgG2 Flex Set by evaluating ten replicates of three different sample levels (inter-assay) and two replicates of three different sample levels from four separate experiments (intra-assay) respectively.

Sample Dilution	Human IgG2	
	Detected (ng/ml)	% of Expected
Starting Dilution	1151.3	101%
1 : 2	551.8	97%
1 : 4	260.8	92%
1 : 8	119.9	84%

**Linearity:** The International Reference Preparation for proteins in human serum, certified reference material 470 (CRM 470), was diluted to the starting dilution (1,139 ng/ml) and serially diluted. The diluted sample was assayed and the results were compared with the original expected concentration.

## Product Notices

- Source of all serum proteins is from USDA inspected abattoirs located in the United States.
- ProClin is a trademark of Rohm and Haas Company.
- This product contains human blood, serum, cells, or materials derived from them, which are potentially hazardous materials. Use universal precautions when handling. Handle as if product were capable of transmitting disease. Material used in this product has been tested using FDA approved methods and found negative for Human Immunodeficiency Virus (HIV-1/HIV-2), Hepatitis B Surface Antigen (HBSAG) and antibody to Hepatitis C Virus (HCV). However, no known test method can offer complete assurance that specimens of human origin will not transmit infectious disease. When handling or disposing, follow precautions described in CDC and FDA recommendations and OSHA Bloodborne Pathogen recommendations.
- Caution: Sodium azide yields highly toxic hydrazoic acid under acidic conditions. Dilute azide compounds in running water before discarding to avoid accumulation of potentially explosive deposits in plumbing.
- Warning: CBA lyophilized standard contains 0.02% (w/w) of a CMIT/MIT mixture (3:1), which is a mixture of: 5-chloro-2-methyl-4-isothiazolin-3-one [EC No 247-500-7] and 2-methyl-4-isothiazolin-3-one [EC No 220-239-6] (3:1).  
Hazard statement: May cause an allergic skin reaction.  
Precautionary statements: Wear protective gloves/eye protection. Wear protective clothing. Avoid breathing mist/vapours/spray. If skin irritation or rash occurs: Get medical advice/attention. IF ON SKIN: Wash with plenty of water. Dispose of contents/container in accordance with local/regional/national/international regulations.

## BD Biosciences

[bdbiosciences.com](http://bdbiosciences.com)

United States	Canada	Europe	Japan	Asia Pacific	Latin America/Caribbean
877.232.8995	800.268.5430	32.2.400.98.95	0120.8555.90	65.6861.0633	55.11.5185.9995

For country contact information, visit [bdbiosciences.com/contact](http://bdbiosciences.com/contact)

*Conditions: The information disclosed herein is not to be construed as a recommendation to use the above product in violation of any patents. BD Biosciences will not be held responsible for patent infringement or other violations that may occur with the use of our products. Purchase does not include or carry any right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of Becton, Dickinson and Company is strictly prohibited.*

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Not for resale.

Unless otherwise noted, BD, BD Logo and all other trademarks are property of Becton, Dickinson and Company. © 2014 BD

