



Anti-ANT Mitoprofile® Antibody

CATALOG #:	457525
COMPONENTS:	250 µg monoclonal antibody irreversibly crosslinked to protein G-agarose beads
APPLICATIONS:	Immunoprecipitation
CLONE ID OF MONOCLONAL ANTIBODY (mAb):	5F51BB5AG7
SPECIES CROSS-REACTIVITY:	human and bovine
HOST SPECIES AND ISOTYPE:	Mouse IgG1, k
IMMUNOGEN:	Recombinant Human ANT
CONCENTRATION:	250 µg of capture antibody crosslinked to 25 µL matrix in 400 µL Phosphate-Buffered Saline (PBS) with 0.02% azide as a preservative.
SUGGESTED WORKING CONCENTRATION:	10 µL matrix can be used to capture ANT from 1 mg solubilized heart mitochondria.
mAb PURITY:	Near homogeneity as judged by SDS-PAGE. The antibody was produced <i>in vitro</i> using hybridomas grown in serum-free medium, and then purified by biochemical fractionation.
STORAGE CONDITIONS:	Store at 4°C. Do not freeze.
COUNTRY OF ORIGIN:	USA

BACKGROUND:

ANT is a reversible transporter of ATP and ADP. During oxidative phosphorylation (OXPHOS) the protein exchanges ATP out for ADP in, however, in the absence of OXPHOS ANT, works in reverse to maintain mitochondrial membrane potential. A subset of patients with heart related diseases have been shown to harbor mutations in the ANT gene or to develop an autoimmune reaction against the protein.

There are a number of proteins found in mitochondria that, under circumstances favoring apoptosis, coalesce to form the so-called permeability transition pore.

The proteins identified as a part of the PTP include cytosolic hexokinase, outer membrane porin (also called the voltage dependent anion channel or VDAC), adenylate cyclase in the intermembrane space, the adenine nucleotide transporter (ANT) and the peripheral benzodiazepine receptor protein of the inner membrane along with cyclophilin D of the matrix space. Hexokinase, porin and ANT all occur as isoforms and it remains to be determined whether there is specificity of these different forms for the PTP.

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.



Related Products

<i>Product</i>	<i>Conjugate</i>	<i>Cat. No.</i>
Protein A	Sepharose 4B	10-1041
rec-Protein G	Sepharose 4B	10-1241
ZyMAX™ Goat anti-rabbit IgG	Unconjugated	81-6100
ZyMAX™ Goat anti-mouse IgG	Unconjugated	81-6500

Secondary Antibody Conjugates

<i>Conjugate</i>	<i>Goat anti-rabbit IgG (H+L)</i>	<i>Goat anti-mouse IgG (H+L)</i>	<i>Ex/Em*</i>	<i>Fluorescence similar to--</i>
Alexa Fluor® 488	A11008	A11001	495/519	FITC
Alexa Fluor® 555	A21428	A21422	555/565	Cy3
Alexa Fluor® 594	A11012	A11005	590/617	Texas Red
Alexa Fluor® 647	A21244	A21235	650/668	Cy5
HRP	81-6120	81-6520	NA**	NA
AP	81-6122	81-6522	NA	NA
Biotin	B2770	B2763	NA	NA

*Excitation/emission (nm); **Not applicable

For additional secondary antibody conjugates, visit www.invitrogen.com/antibodies

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.

Immunocapture Protocol

MATERIALS REQUIRED

Reagents:

1. MitoSciences immunocapture antibody coupled to agarose beads
2. n-dodecyl- β -D-maltopyranoside (Lauryl maltoside, MitoSciences MS910)
3. Phosphate buffered saline, PBS (recipe see Page 6)
4. Elution buffer – Glycine, SDS or Urea elution buffer (Page 6)
5. Protease inhibitor cocktail (Page 6)
6. Double distilled water

Equipment:

1. Laboratory benchtop microfuge
2. Protein electrophoresis equipment
3. Tube rotation equipment
4. pH meter, weighing balance and other standard lab equipment

SAMPLE PREPARATION

When performing an immunocapture procedure, it is always recommended to isolate mitochondria from cells before immunoprecipitation. Procedures for mitochondrial isolation can be found at www.mitosciences.com/PDF/mitos.pdf

It is possible, however, to isolate complexes from whole tissue or cell extract, although this may result in a weaker signal and/or additional bands resulting from non-specific cross-reactivity.

MitoSciences' immunocapture antibodies have been optimized to immunoprecipitate the OXPHOS and PDH complexes from a wide range species. However a minimal amount of starting mitochondria/cells is critical. Suggested minimum amounts of mitochondria as starting material are presented in Table 1 providing the user with the opportunity to generate the best quality product.

SAMPLE	MINIMAL STARTING AMOUNT	RECOMMENDED STARTING AMOUNT
Heart mitochondria	100 μ g	1-5 mg
Muscle mitochondria	200 μ g	2-5 mg
Brain mitochondria	300 μ g	5 mg
Cultured cell mitochondria	1 mg	5 mg
Cultured cell extract	6 mg	15 mg

Table 1. Suggested minimal starting amounts.



The total amount of OXPHOS complexes in mitochondrial samples varies greatly between species and tissue types. Therefore it is highly recommended that during the experimental planning steps an estimation is made of the total amount of the complex in the user's sample. In this way the appropriate detection strategy can then be employed. Table 2 suggests detection strategies based upon anticipated yield of immunocaptured product.

YIELD OF COMPLEX	DETECTION STRATEGY
1 µg +	Gel staining with Coomassie
10 ng +	Gel staining with silver/sypro ruby
1 ng +	Western blotting with MitoSciences mAbs
Any	Mass spectrometry

Table 2. Suggested detection methods by yield of product.

SAMPLE SOLUBILIZATION

The sample should be solubilized in a non-ionic detergent. It has been determined that at a protein concentration of 5 mg/mL mitochondria are completely solubilized by 20 mM n-dodecyl-β-D-malto-pyranoside (1% w/v lauryl maltoside). The key to this solubilization process is that the membranes are disrupted while the previously membrane embedded multisubunit OXPHOS complexes remain intact, a step necessary for the antibody based purification procedure described below.*

1. To a mitochondrial membrane suspension at 5.5 mg/mL protein in PBS add 1/10 volume of 10% lauryl maltoside (final concentration of 1%).
2. Mix well and incubate on ice for 30 minutes.
3. Centrifuge at 72,000 g for 30 minutes. The Beckman Optima benchtop ultracentrifuge is recommended for small sample volumes ** (At a minimum, a benchtop microfuge on maximum speed, usually around 16,000 g should suffice).
4. Collect the supernatant and discard the pellet.

Note: Samples rich in mitochondria such as heart mitochondria, the cytochromes in Complexes II and III should give this supernatant a brown coloration.

5. Add a protease inhibitor cocktail to the mixture (see Page 6) and keep the sample on ice until immunoprecipitation is performed.

Note: One important exception to this solubilization method is the pyruvate dehydrogenase enzyme. In order to isolate PDH at a protein concentration of 5 mg/mL mitochondria the required detergent concentration is only 10 mM (0.5%) lauryl maltoside.

The PDH enzyme should also be centrifuged at lower speed, a centrifugal force of 16,000 g is maximum for the PDH complex.

IMMUNOPRECIPITATION

MitoSciences' immunocapture beads are agarose beads irreversibly cross-linked to highly specific monoclonal antibodies, which are capable of binding and retaining specific OXPHOS complexes or the PDH complex. The loaded beads are completely saturated with antibody to ensure the maximum amount of antibody per bead volume and hence the maximum amount of immunoprecipitated product.

The smallest working amount of beads is around 5 μ L of solid beads in a small microtube (e.g. a 500 μ L tube). It is not practical to use a volume smaller than this for immunocapture procedure, therefore it is recommended that when wishing to use less beads researchers dilute the concentrated MitoSciences' beads with unloaded agarose beads, giving a workable volume of beads. The yield from such diluted beads will of course be less. Plain beads for dilution are available from MitoSciences.

As an alternative each immunocapture antibody, free in solution i.e. unbound to agarose beads, is also available from MitoSciences.

1. Add the desired amount of antibody loaded agarose beads (i.e. at least 5 μ L of the solid beads) to the appropriate amount of solubilized mitochondrial supernatant.
2. Allow this mixture to mix for at least 3 hours at room temperature or overnight at 4°C. Mixing should be done on a nutator, or by turning in a tube rotator such as the one shown below.



ELUTION

1. After the mixing step is complete, collect the beads by centrifugation for 1 minute at a slow speed (i.e. 1,000-3,000g or the slowest setting on most benchtop microfuges).
2. Remove the *supernatant* from above the beads and discard. The complex of interest should now be specifically bound to the antibody coating the beads.
3. Wash the beads to remove any non-specifically bound proteins prior to elution by adding 100 volumes of wash buffer (see Page 6) to the beads.
4. Gently mix for 5 minutes. Collect the beads by gentle centrifugation as performed in Step 1.
5. Remove the wash buffer from above the beads only and discard. Repeat bead washing process twice.
6. In the final step, all wash buffer is removed from above the beads. The complex is now ready for elution from beads collected in the bottom of the tube.

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com


PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.

Three options are available for elution of the bound complex from the beads. The chosen elution procedure should be performed on the beads three times. This ensures complete removal of target from the beads. The three samples should be collected and analyzed, samples containing the most protein should then be pooled. Possible elution methods are:

- (1) **Glycine buffer elution** – the complex is eluted from the beads by acidification. Beads are resuspended in 2-5 volumes of glycine elution buffer (pH 2.0) – see Page 6. This mixture is incubated for 10 minutes with frequent agitation before gentle centrifugation. The purified complexes have now been released into the supernatant which should be collected from *above* the beads *only*. It is advised to repeat this process with fresh glycine buffer each time at least twice more to ensure that all of the captured complex has been released from the beads. The eluted sample has an acidic pH which may need to be neutralized before analysis – see Troubleshooting guide. This method is ADVANTAGEOUS because the beads may be reused after thorough elution and removal of glycine elution buffer. To do this, wash the beads by adding 1 ml of PBS. Collect the beads by centrifugation and pipette off the PBS. Repeat this wash step. The beads may now be reused.
- (2) **SDS buffer elution** – the complex is eluted from the beads by the denaturant SDS. Beads are resuspended in 2-5 volumes of SDS elution buffer– see Page 6. This mixture is incubated for 10 minutes with frequent agitation **before** gentle centrifugation. The purified complexes have now been released into the supernatant which should be collected from *above* the beads *only*. It is advised to repeat this process at least one more time to ensure all of the captured complex has been released from the beads. This method is ADVANTAGEOUS because the extraction method is highly efficient and therefore the sample is more concentrated. However the antibody is denatured by the SDS and is no longer viable and should be discarded.
- (3) **Urea buffer elution** - the complex is eluted from the beads by the chaotrope urea. Beads are resuspended in 2-5 volumes of urea elution buffer – see Page 6. This mixture is incubated for 10 minutes with frequent agitation before gentle centrifugation. The purified complexes have now been released into the supernatant which should be collected from *above* the beads *only*. It is advised to repeat this process at least twice more to ensure that all of the captured complex has been released from the beads. This is ADVANTAGEOUS because the sample may be digested by proteolytic enzymes for mass spectrometry. However the sample should be diluted at least four fold in order to reduce the urea concentration to levels permitting proteolysis by trypsin – see page 7.

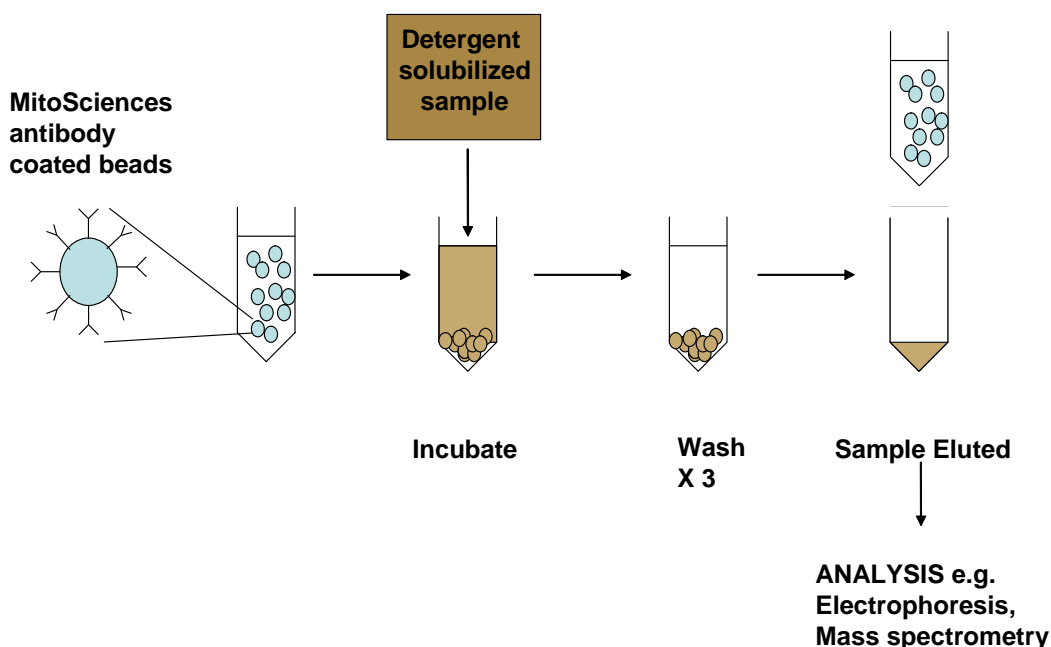

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.



SAMPLE ANALYSIS

Samples eluted by any of the three methods can now be resolved by electrophoresis. Resolved proteins should be detected by the method chosen in Table II on Page 2. Optimized protocols for electrophoresis, gel staining and Western blotting can be found at www.mitosciences.com/PDF/western.pdf. As described in these protocols samples are first solubilized in SDS-PAGE sample buffer.

No antibody should be present in the sample once eluted from the beads; therefore prior to loading, the sample can be reduced by a reducing agent such as 50 mM DTT or 1% β -mercaptoethanol. Another optional step is heating of the sample which can be done at 95°C for 5 minutes or at 37°C for 30 minutes prior to loading onto the gel. *These steps may increase the resolution of protein bands and also reduce the complexity of the sample by breaking any disulfide bonded proteins.*

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.

BUFFER RECIPES

Phosphate buffered saline solution (PBS)

1.4 mM KH_2PO_4
8 mM Na_2HPO_4
140 mM NaCl
2.7 mM KCl, pH 7.3

Lauryl maltoside stock

200 mM n-dodecyl- β -D-maltopyranoside (10% w/v lauryl maltoside), (Anatrace D310S)

1000 x Protease inhibitor stocks

1 M phenylmethanesulfonyl fluoride (PMSF) in acetone (Sigma L7626)
1 mg/mL leupeptin (Sigma L2884)
1 mg/mL pepstatin (Sigma P4265)

Alternatively, concentrated pre-formulated protease cocktails are available (Sigma P8340)

Bead wash buffer

1x PBS
1 mM n-dodecyl- β -D-maltopyranoside (0.05% w/v lauryl maltoside)

Glycine elution buffer

0.2 M Glycine. HCl pH 2.5
1 mM n-dodecyl- β -D-maltopyranoside (0.05% w/v lauryl maltoside)

SDS elution buffer

1% sodium dodecyl sulfate (SDS) (Sigma L4509)

Urea elution buffer

4 M Urea. HCl pH 7.5 (Sigma U1250)

2x SDS page sample buffer

20% glycerol
4% SDS
100 mM Tris pH 6.8
0.002% Bromophenol blue
optional – 100 mM dithiothreitol

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.



OPTIMIZATION STEPS AND GENERAL TIPS

Using agarose bead slurries

Since the beads are a solid material they cannot be pipetted directly. Instead they are provided in a much larger volume of liquid (usually 40 volumes of PBS). Pipetting this solution up and down mixes the beads into a slurry allowing their transfer to the experimental tube. Since bead losses can occur on the inside of the *pipette tip* this is the only time in this protocol the beads are pipetted directly. All other steps in this protocol require sample mixing by rotation or mixing by in a large volume of buffer. Therefore the beads should not be mixed by pipetting to avoid losses. Also, avoid vigorous mixing during the elution step when the liquid volume is low since beads might become deposited around the inside tube unexposed to elution buffer leading to losses. Instead gently tap the tube to agitate the beads within the small volume of sample elution buffer.

Samples eluted by Glycine buffer

Sample eluted by glycine buffer are low in pH. In most cases it is necessary to remove this acidity with a strong buffer. For example, adding SDS-PAGE loading buffer directly to a glycine eluted sample will turn this sample from blue to a yellow as the bromophenol blue acts as a pH indicator. Therefore the sample should be neutralized by the slow addition a 1 M Tris.HCl pH 7.5 in microliter amounts until blue color is restored.

Sample concentration

When analyzing immunocaptured products by SDS-PAGE, it is recommended to load as much sample as possible on the gel. Samples may also be supplemented with fresh reducing agent such as dithiothreitol or β -mercaptoethanol. Heating samples at 95°C for 5 minutes or at 37°C for 30 minutes is also optional.

Blot development

When analyzing immunocaptured products by Western blotting choose an appropriate method for blot development. The alkaline phosphatase (NBT/BCIP) and horseradish peroxidase (ECL) methods are recommended.

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089


Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.

TROUBLESHOOTING GUIDE

Antibody contamination	<p>When eluting pipette only the liquid sample from above the beads. This sample can be spun again and aspirated to ensure that it is free of beads</p> <p>Electrophoresis- Do not include reducing agent in sample during electrophoresis, this should maintain antibody at 200 kDa during electrophoresis</p> <p>Western blotting – Change secondary to TrueBlot to reduce cross reactivity with immunocapture antibody. (www.eBiosciences.com)</p>
Sample turns yellow with loading buffer addition	Neutralize the acidity with Tris Base
Weak or no signal	<p>Increase the bead amount</p> <p>Isolate mitochondria from the sample</p> <p>Increase the amount of sample</p> <p>Increase sample/bead incubation time</p>
Non-specific bands	<p>Isolate mitochondria to higher purity</p> <p>Add a reducing agent to the eluted sample e.g. DTT</p> <p>Heat the eluted sample at 95°C for 5 min before loading</p>

FLOW CHART

This guide is for quick reference only. Be completely familiar with the previous details of this document before performing the assay.

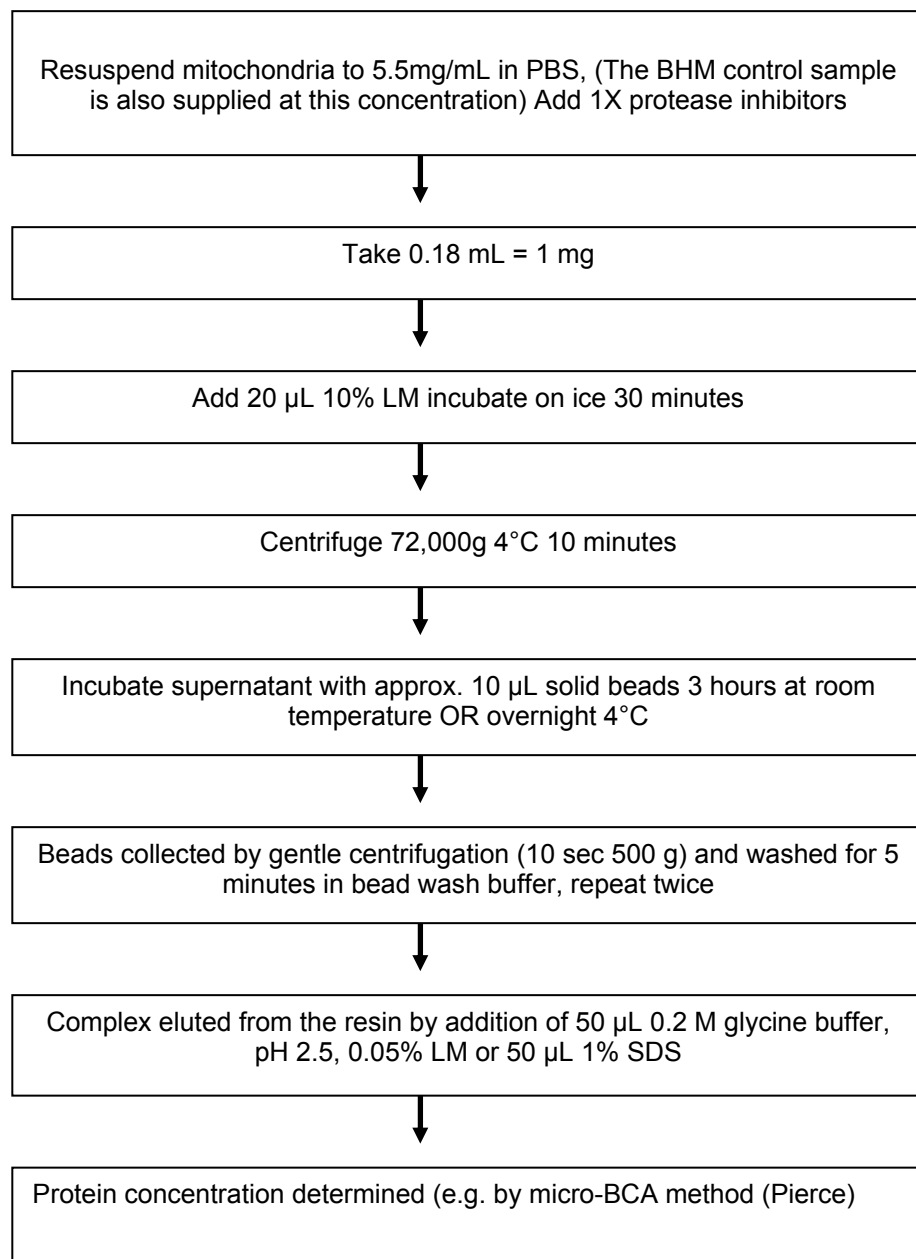

For Research Use Only



Manufactured exclusively for Invitrogen by MitoSciences, Inc.

www.invitrogen.com

Invitrogen Corporation • 542 Flynn Rd • Camarillo • CA 93012 • Tel: 800.955.6288 • E-mail: techsupport@invitrogen.com

PI457525

(Rev 10/08) DCC-08-1089

Important Licensing Information - These products may be covered by one or more Limited Use Label Licenses (see the Invitrogen Catalog or our website, www.invitrogen.com). By use of these products you accept the terms and conditions of all applicable Limited Use Label Licenses. Unless otherwise indicated, these products are for research use only and are not intended for human or animal diagnostic, therapeutic or commercial use.