

# CD45 antibodies, mouse

## For research use only

30 µg equal 100 tests, 150 µg equal 500 tests. One test corresponds to labeling of 10<sup>6</sup> cells.

Product	Content	Order no.
CD45-Biotin	30 µg in 200 µL	130-110-795
CD45-FITC	30 µg in 200 µL	130-110-796
CD45-FITC	4x150 µg in 1 mL	130-110-658
CD45-PE	30 µg in 200 µL	130-110-797
CD45-PE	2x150 µg in 1 mL	130-110-659
CD45-APC	30 µg in 200 µL	130-110-798
CD45-APC	150 µg in 1 mL	130-110-660
CD45-VioBlue	30 µg in 200 µL	130-110-802
CD45-VioBlue	150 µg in 1 mL	130-110-664
CD45-VioGreen	30 µg in 200 µL	130-110-803
CD45-VioGreen	150 µg in 1 mL	130-110-665
CD45-PE-Vio615	30 µg in 200 µL	130-110-804
CD45-PE-Vio615	150 µg in 1 mL	130-110-666
CD45-PE-Vio770	30 µg in 200 µL	130-110-799
CD45-PE-Vio770	150 µg in 1 mL	130-110-661
CD45-APC-Vio770	30 µg in 200 µL	130-110-800
CD45-APC-Vio770	150 µg in 1 mL	130-110-662
CD45-PerCP-Vio700	30 µg in 200 µL	130-110-801
CD45-PerCP-Vio700	150 µg in 1 mL	130-110-663
CD45-Biotin	4x150 µg in 1 mL	130-110-657

## Warnings

Reagents contain sodium azide. Under acidic conditions sodium azide yields hydrazoic acid, which is extremely toxic. Azide compounds should be diluted with running water before discarding. These precautions are recommended to avoid deposits in plumbing where explosive conditions may develop.

## Technical data and background information

<b>Antigen</b>	CD45
<b>Clone</b>	REA737
<b>Isotype</b>	recombinant human IgG1
<b>Isotype control</b>	REA Control antibodies
<b>Alternative names of antigen</b>	L-CA, LCA, Ly-5, T200

<b>Entrez Gene ID</b>	<a href="#">19264</a>
<b>Molecular mass of antigen [kDa]</b>	142
<b>Distribution of antigen</b>	T cells, B cells
<b>Product format</b>	Reagents are supplied in buffer containing stabilizer and 0.05% sodium azide.
<b>Fixation</b>	Cells should be stained prior to fixation, if formaldehyde is used as a fixative.
<b>Storage</b>	Store protected from light at 2–8 °C. Do not freeze.

Clone REA737 recognizes the mouse CD45 antigen, also known as Ly-5 or leukocyte common antigen (LCA), which belongs to the protein tyrosine phosphatase (PTP) family. CD45 is a glycoprotein which is involved in T cell receptor and B cell receptor signal transduction. It is expressed at high levels on all cells of hematopoietic origin except for erythrocytes. Clone REA737 reacts with all CD45 isoforms. CD45 can be used to discriminate leukocytes from non-hematopoietic cells. Additional information: Clone REA737 displays negligible binding to Fc receptors.

## Reagent requirements











- Buffer: Prepare a solution containing phosphate-buffered saline (PBS), pH 7.2, 0.5% bovine serum albumin (BSA), and 2 mM EDTA by diluting MACS<sup>®</sup> BSA Stock Solution (# 130-091-376) 1:20 with autoMACS<sup>®</sup> Rinsing Solution (# 130-091-222). Keep buffer cold (2–8 °C).  
Note: EDTA can be replaced by other supplements such as anticoagulant citrate dextrose formula-A (ACD-A) or citrate phosphate dextrose (CPD). Buffers or media containing Ca<sup>2+</sup> or Mg<sup>2+</sup> are not recommended for use.
- (Optional) Fluorochrome-conjugated anti-biotin antibodies, e.g., Anti-Biotin-PE (# 130-090-756) as secondary antibody reagent in combination with biotinylated antibodies.
- (Optional) Propidium Iodide Solution (# 130-093-233) for flow cytometric exclusion of dead cells without fixation.
- (Optional) Fixation and Dead Cell Discrimination Kit (# 130-091-163) for cell fixation and flow cytometric exclusion of dead cells.











## Protocol for cell surface staining

- The recommended antibody dilution for labeling of cells and subsequent analysis by flow cytometry is 1:50 for up to 10<sup>6</sup> cells/100 µL.
  - Volumes given below are for up to 10<sup>6</sup> nucleated cells. When working with fewer than 10<sup>6</sup> cells, use the same volumes as indicated. When working with higher cell numbers, scale up all reagent volumes and total volumes accordingly.
1. Determine cell number.
  2. Centrifuge cell suspension at 300×g for 10 minutes. Aspirate supernatant completely.
  3. Resuspend up to 10<sup>6</sup> nucleated cells per 98 µL of buffer.
  4. Add 2 µL of the antibody.
  5. Mix well and incubate for 10 minutes in the dark in the refrigerator (2–8 °C).  
Note: Higher temperatures and/or longer incubation times may lead to non-specific cell labeling. Working on ice requires increased incubation times.
  6. Wash cells by adding 1–2 mL of buffer and centrifuge at 300×g for 10 minutes. Aspirate supernatant completely.
  7. (Optional) If biotinylated antibody was used, resuspend the cell pellet in buffer and stain with fluorochrome-conjugated anti-biotin antibody according to the manufacturer's recommendations.
  8. Resuspend cell pellet in a suitable amount of buffer for analysis by flow cytometry or fluorescence microscopy.

## Examples of immunofluorescent staining

Splenocytes from C57BL/6 mice were stained with CD45 antibodies or with the corresponding REA Control antibodies (left image). Flow cytometry was performed using the MACSQuant<sup>®</sup> Analyzer. Cell debris and dead cells were excluded from the analysis based on scatter signals and propidium iodide fluorescence or 4',6-diamidino-2-phenylindole (DAPI) fluorescence, as in the case of tandem conjugates.

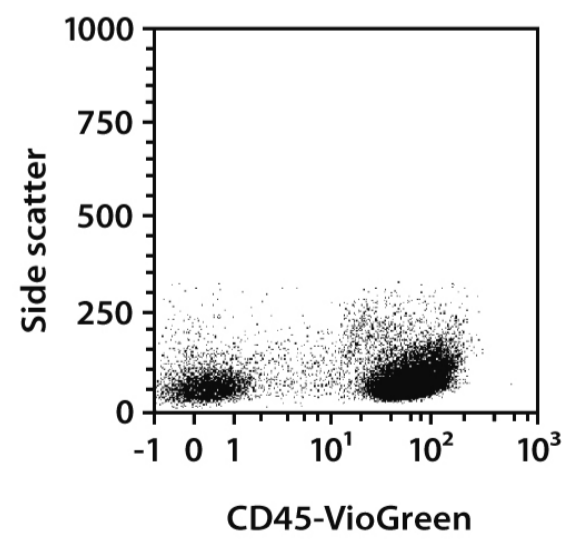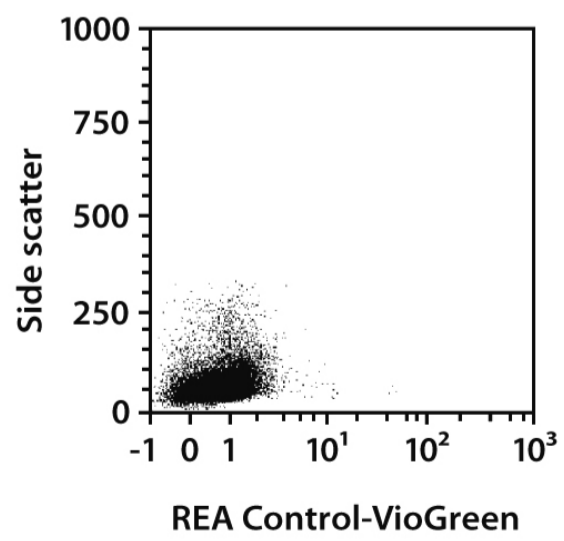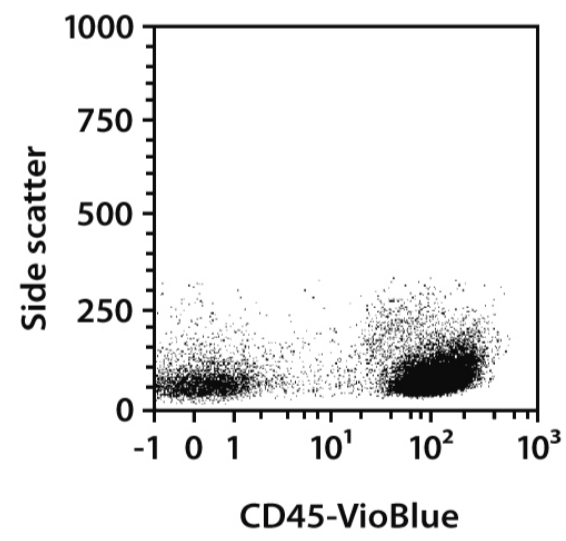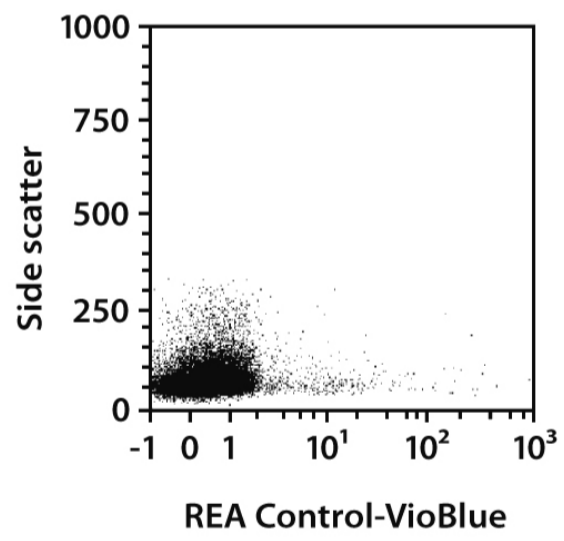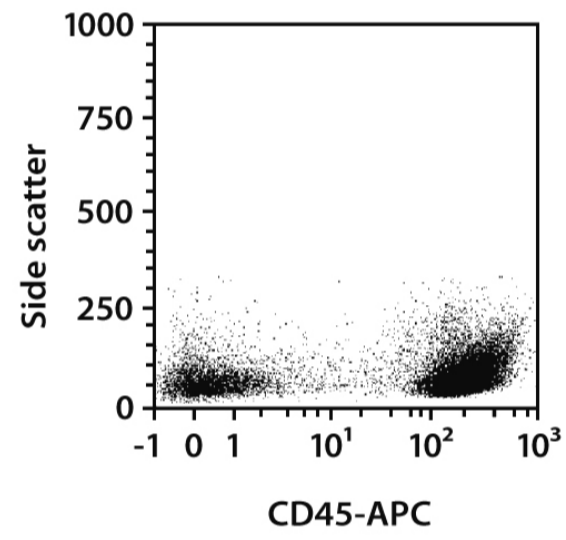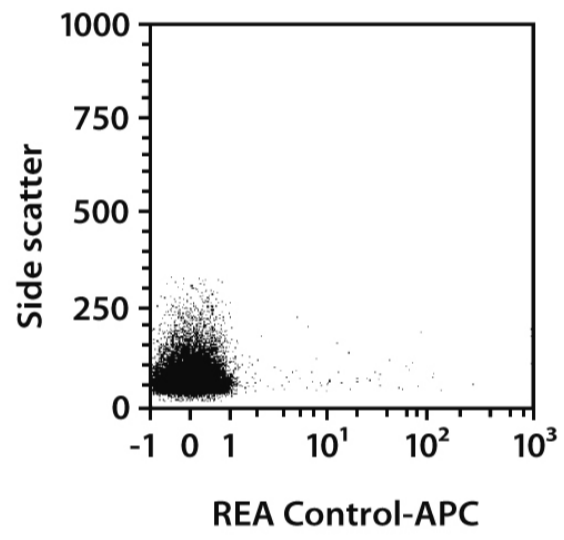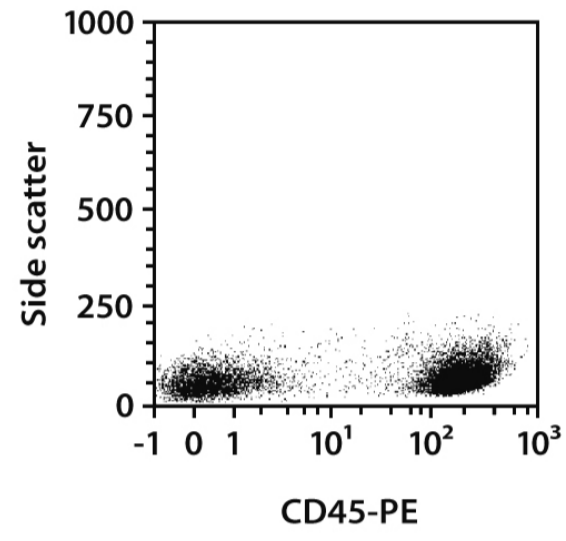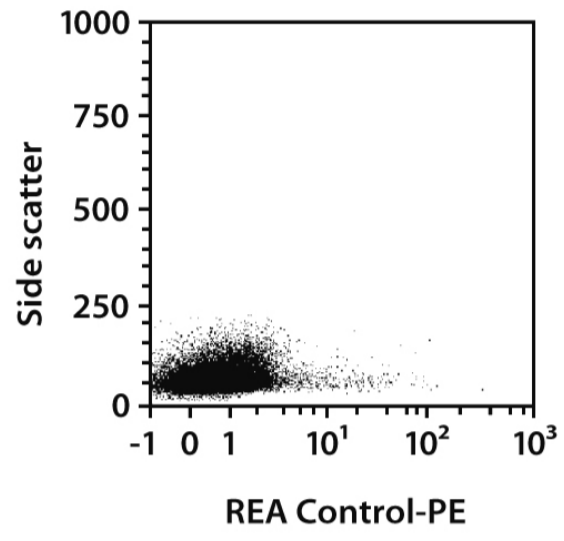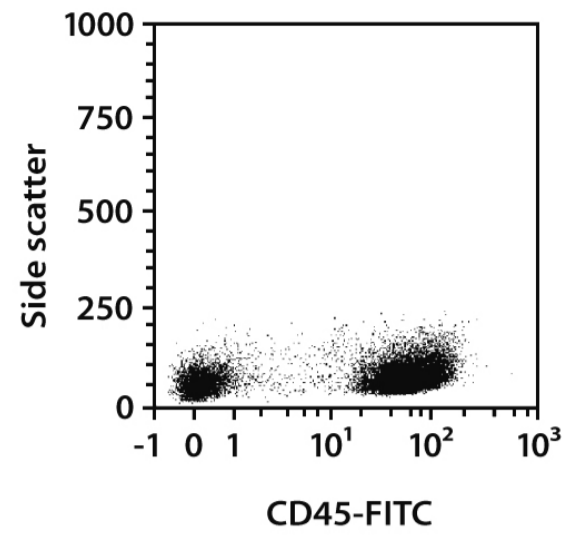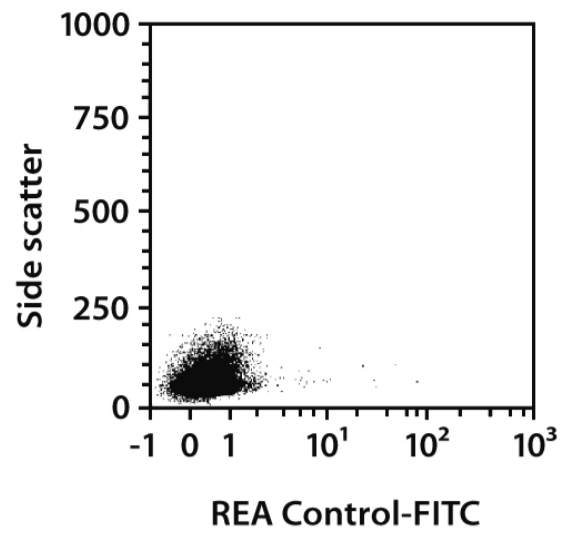

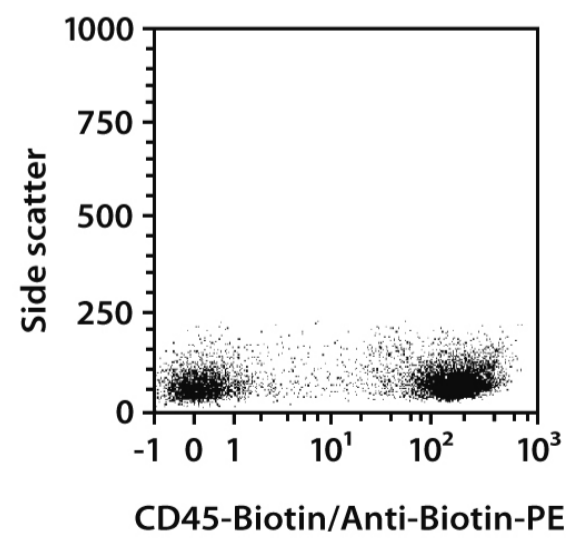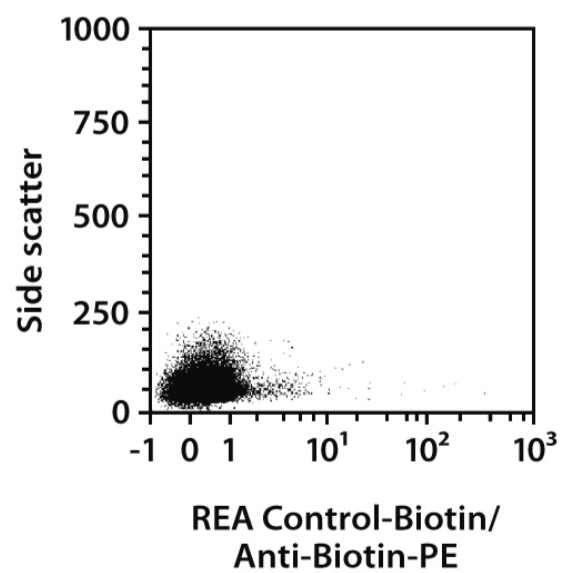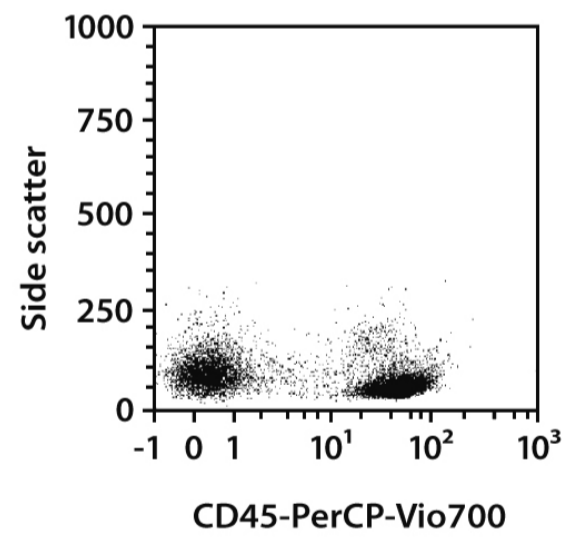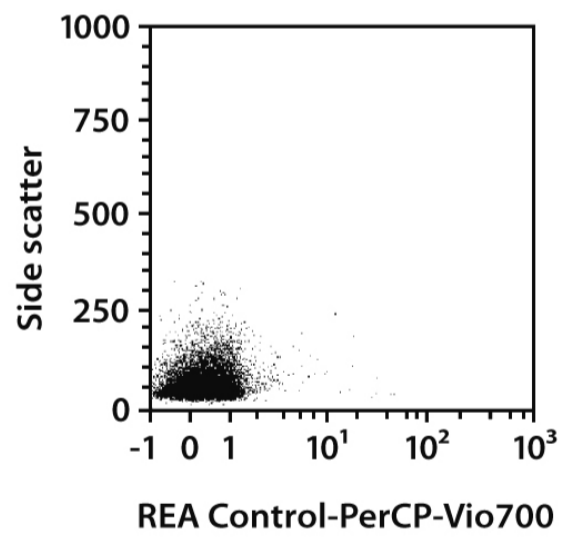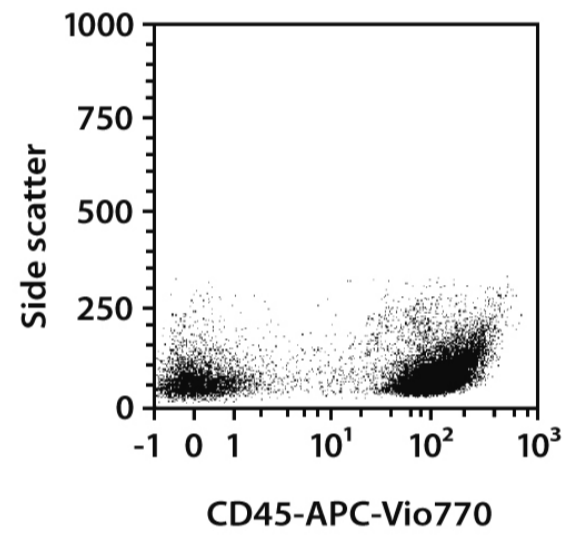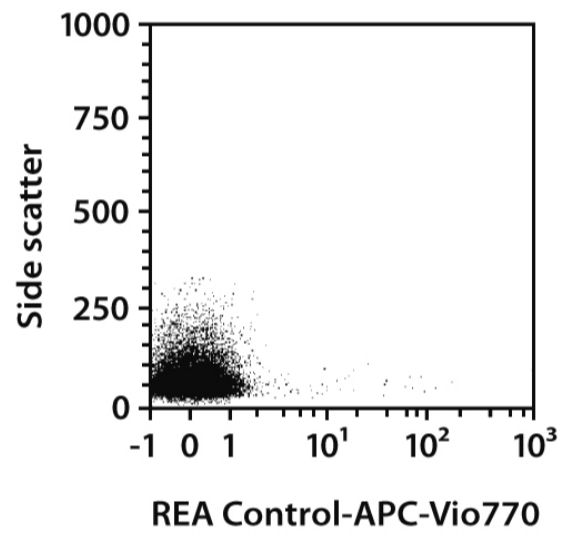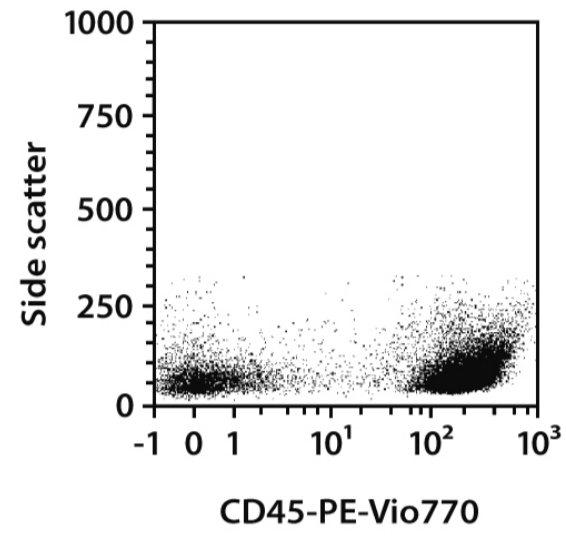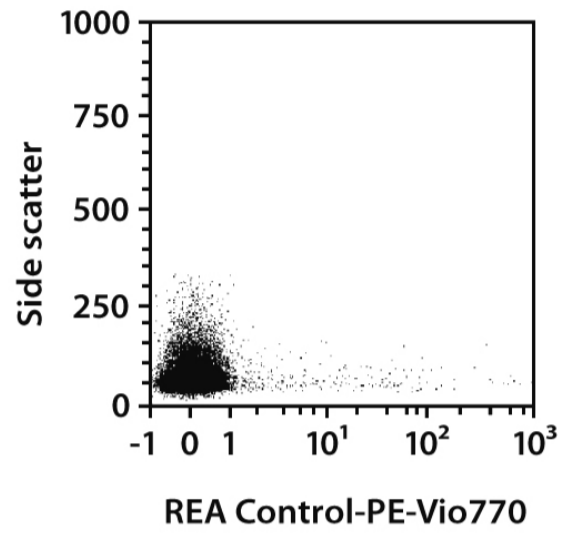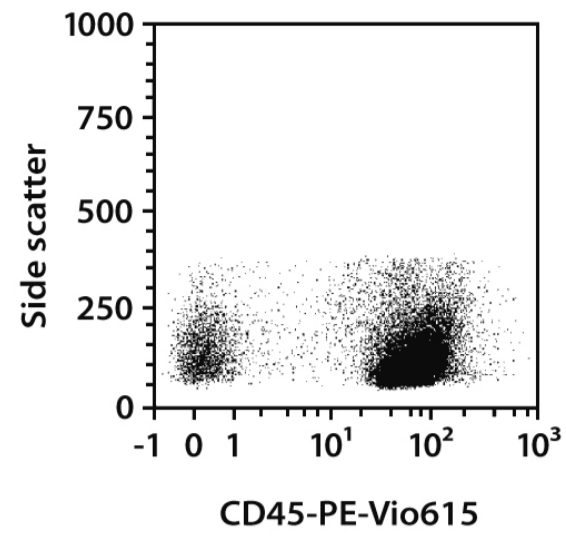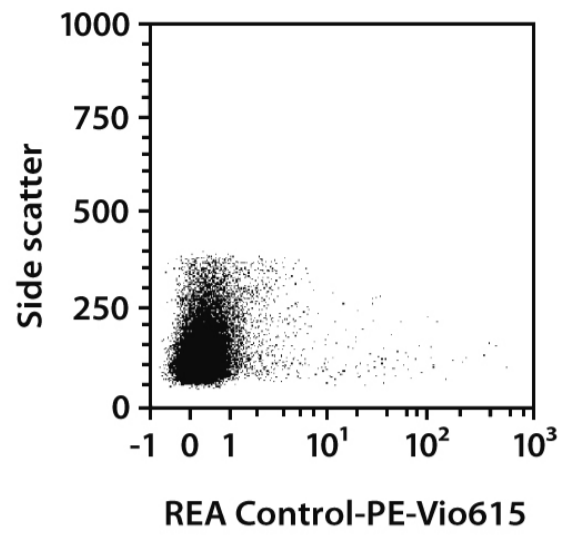

## Warranty

The products sold hereunder are warranted only to be free from defects in workmanship and material at the time of delivery to the customer. Miltenyi Biotec GmbH makes no warranty or representation, either expressed or implied, with respect to the fitness of a product for a particular purpose. There are no warranties, expressed or implied, which extend beyond the technical specifications of the products. Miltenyi Biotec GmbH's liability is limited to either replacement of the products or refund of the purchase price. Miltenyi Biotec GmbH is not liable for any property damage, personal injury or economic loss caused by the product.

**Miltenyi Biotec GmbH** | Friedrich-Ebert-Straße 68 | 51429 Bergisch Gladbach | Germany | Phone +49 2204 8306-0 | Fax +49 2204 85197 | macs@miltenyibiotec.de | [www.miltenyibiotec.com](http://www.miltenyibiotec.com) Miltenyi Biotec provides products and services worldwide. Visit [www.miltenyibiotec.com/local](http://www.miltenyibiotec.com/local) to find your nearest Miltenyi Biotec contact.

Unless otherwise specifically indicated, Miltenyi Biotec products and services are for research use only and not for therapeutic or diagnostic use. autoMACS, MACS, MACSQuant, Vio, VioBlue, VioBright, and VioGreen are either trademarks or registered trademarks of Miltenyi Biotec GmbH. Copyright © 2016 Miltenyi Biotec GmbH. All rights reserved.