

Anti-Ter-119 antibodies, mouse

For research use only

30 µg equal 100 tests, 150 µg equal 500 tests. One test corresponds to labeling of 10⁶ cells.

Product	Content	Order no.
Anti-Ter-119-Biotin	150 µg in 1 mL	130-112-718
Anti-Ter-119-FITC	30 µg in 200 µL	130-112-908
Anti-Ter-119-FITC	150 µg in 1 mL	130-112-719
Anti-Ter-119-PE	30 µg in 200 µL	130-112-909
Anti-Ter-119-PE	150 µg in 1 mL	130-112-720
Anti-Ter-119-APC	30 µg in 200 µL	130-112-910
Anti-Ter-119-APC	150 µg in 1 mL	130-112-721
Anti-Ter-119-VioBlue	30 µg in 200 µL	130-112-914
Anti-Ter-119-VioBlue	150 µg in 1 mL	130-112-725
Anti-Ter-119-PE-Vio615	30 µg in 200 µL	130-112-915
Anti-Ter-119-PE-Vio615	150 µg in 1 mL	130-112-726
Anti-Ter-119-PE-Vio770	30 µg in 200 µL	130-112-911
Anti-Ter-119-PE-Vio770	150 µg in 1 mL	130-112-722
Anti-Ter-119-APC-Vio770	30 µg in 200 µL	130-112-912
Anti-Ter-119-APC-Vio770	150 µg in 1 mL	130-112-723
Anti-Ter-119-PerCP-Vio700	30 µg in 200 µL	130-112-913
Anti-Ter-119-PerCP-Vio700	150 µg in 1 mL	130-112-724
Anti-Ter-119-Biotin	30 µg in 200 µL	130-112-907

Warnings

Reagents contain sodium azide. Under acidic conditions sodium azide yields hydrazoic acid, which is extremely toxic. Azide compounds should be diluted with running water before discarding. These precautions are recommended to avoid deposits in plumbing where explosive conditions may develop.

Technical data and background information

Antigen	Ter-119
Clone	REA847
Isotype	recombinant human IgG1
Isotype control	REA Control antibodies
Alternative names of antigen	Ly-76, Ly76
Entrez Gene ID	104231
Distribution of antigen	red blood cells, spleen, bone marrow

Product format	Reagents are supplied in buffer containing stabilizer and 0.05% sodium azide.
Fixation	Cells should be stained prior to fixation, if formaldehyde is used as a fixative.
Storage	Store protected from light at 2–8 °C. Do not freeze.

Clone REA847 recognizes the mouse Ter-119 antigen, a glycoprotein A-associated protein, also known as Ly-76. Ter-119 is expressed on mature erythrocytes and erythroid precursor cells in adult blood, spleen, and bone marrow, as well as in the embryonic yolk sac and fetal liver. REA847 does not react with cells showing typical erythroid blast-forming unit (BFU-E) and erythroid colony-forming unit (CFU-E) activity. In adult mice, REA847 reacts with 20–25% of bone marrow cells and approximately 50% of spleen cells, but not with thymocytes or lymph node cells. Additional information: Clone REA847 displays negligible binding to Fc receptors.

Reagent requirements


- Buffer: Prepare a solution containing phosphate-buffered saline (PBS), pH 7.2, 0.5% bovine serum albumin (BSA), and 2 mM EDTA by diluting MACS[®] BSA Stock Solution (# 130-091-376) 1:20 with autoMACS[®] Rinsing Solution (# 130-091-222). Keep buffer cold (2–8 °C).
Note: EDTA can be replaced by other supplements such as anticoagulant citrate dextrose formula-A (ACD-A) or citrate phosphate dextrose (CPD). Buffers or media containing Ca²⁺ or Mg²⁺ are not recommended for use.
- (Optional) Fluorochrome-conjugated anti-biotin antibodies, e.g., Anti-Biotin-PE (# 130-090-756) as secondary antibody reagent in combination with biotinylated antibodies.
- (Optional) Propidium Iodide Solution (# 130-093-233) for flow cytometric exclusion of dead cells without fixation.
- (Optional) Fixation and Dead Cell Discrimination Kit (# 130-091-163) for cell fixation and flow cytometric exclusion of dead cells.

Protocol for cell surface staining

- The recommended antibody dilution for labeling of cells and subsequent analysis by flow cytometry is 1:50 for up to 10⁶ cells/100 µL.
 - Volumes given below are for up to 10⁶ nucleated cells. When working with fewer than 10⁶ cells, use the same volumes as indicated. When working with higher cell numbers, scale up all reagent volumes and total volumes accordingly.
1. Determine cell number.
 2. Centrifuge cell suspension at 300×g for 10 minutes. Aspirate supernatant completely.
 3. Resuspend up to 10⁶ nucleated cells per 98 µL of buffer.
 4. Add 2 µL of the antibody.
 5. Mix well and incubate for 10 minutes in the dark in the refrigerator (2–8 °C).
Note: Higher temperatures and/or longer incubation times may lead to non-specific cell labeling. Working on ice requires increased incubation times.
 6. Wash cells by adding 1–2 mL of buffer and centrifuge at 300×g for 10 minutes. Aspirate supernatant completely.
 7. (Optional) If biotinylated antibody was used, resuspend the cell pellet in buffer and stain with fluorochrome-conjugated anti-biotin antibody according to the manufacturer's recommendations.
 8. Resuspend cell pellet in a suitable amount of buffer for analysis by flow cytometry or fluorescence microscopy.

Examples of immunofluorescent staining

Splenocytes of C57BL/6 mice were stained with Anti-Ter-119 antibodies or with the corresponding REA Control antibodies (left peak). Flow cytometry was performed using the MACSQuant[®] Analyzer. Cell debris and dead cells were excluded from the analysis based on scatter signals and propidium iodide fluorescence or 4',6-diamidino-2-phenylindole (DAPI) fluorescence, as in the case of tandem conjugates.

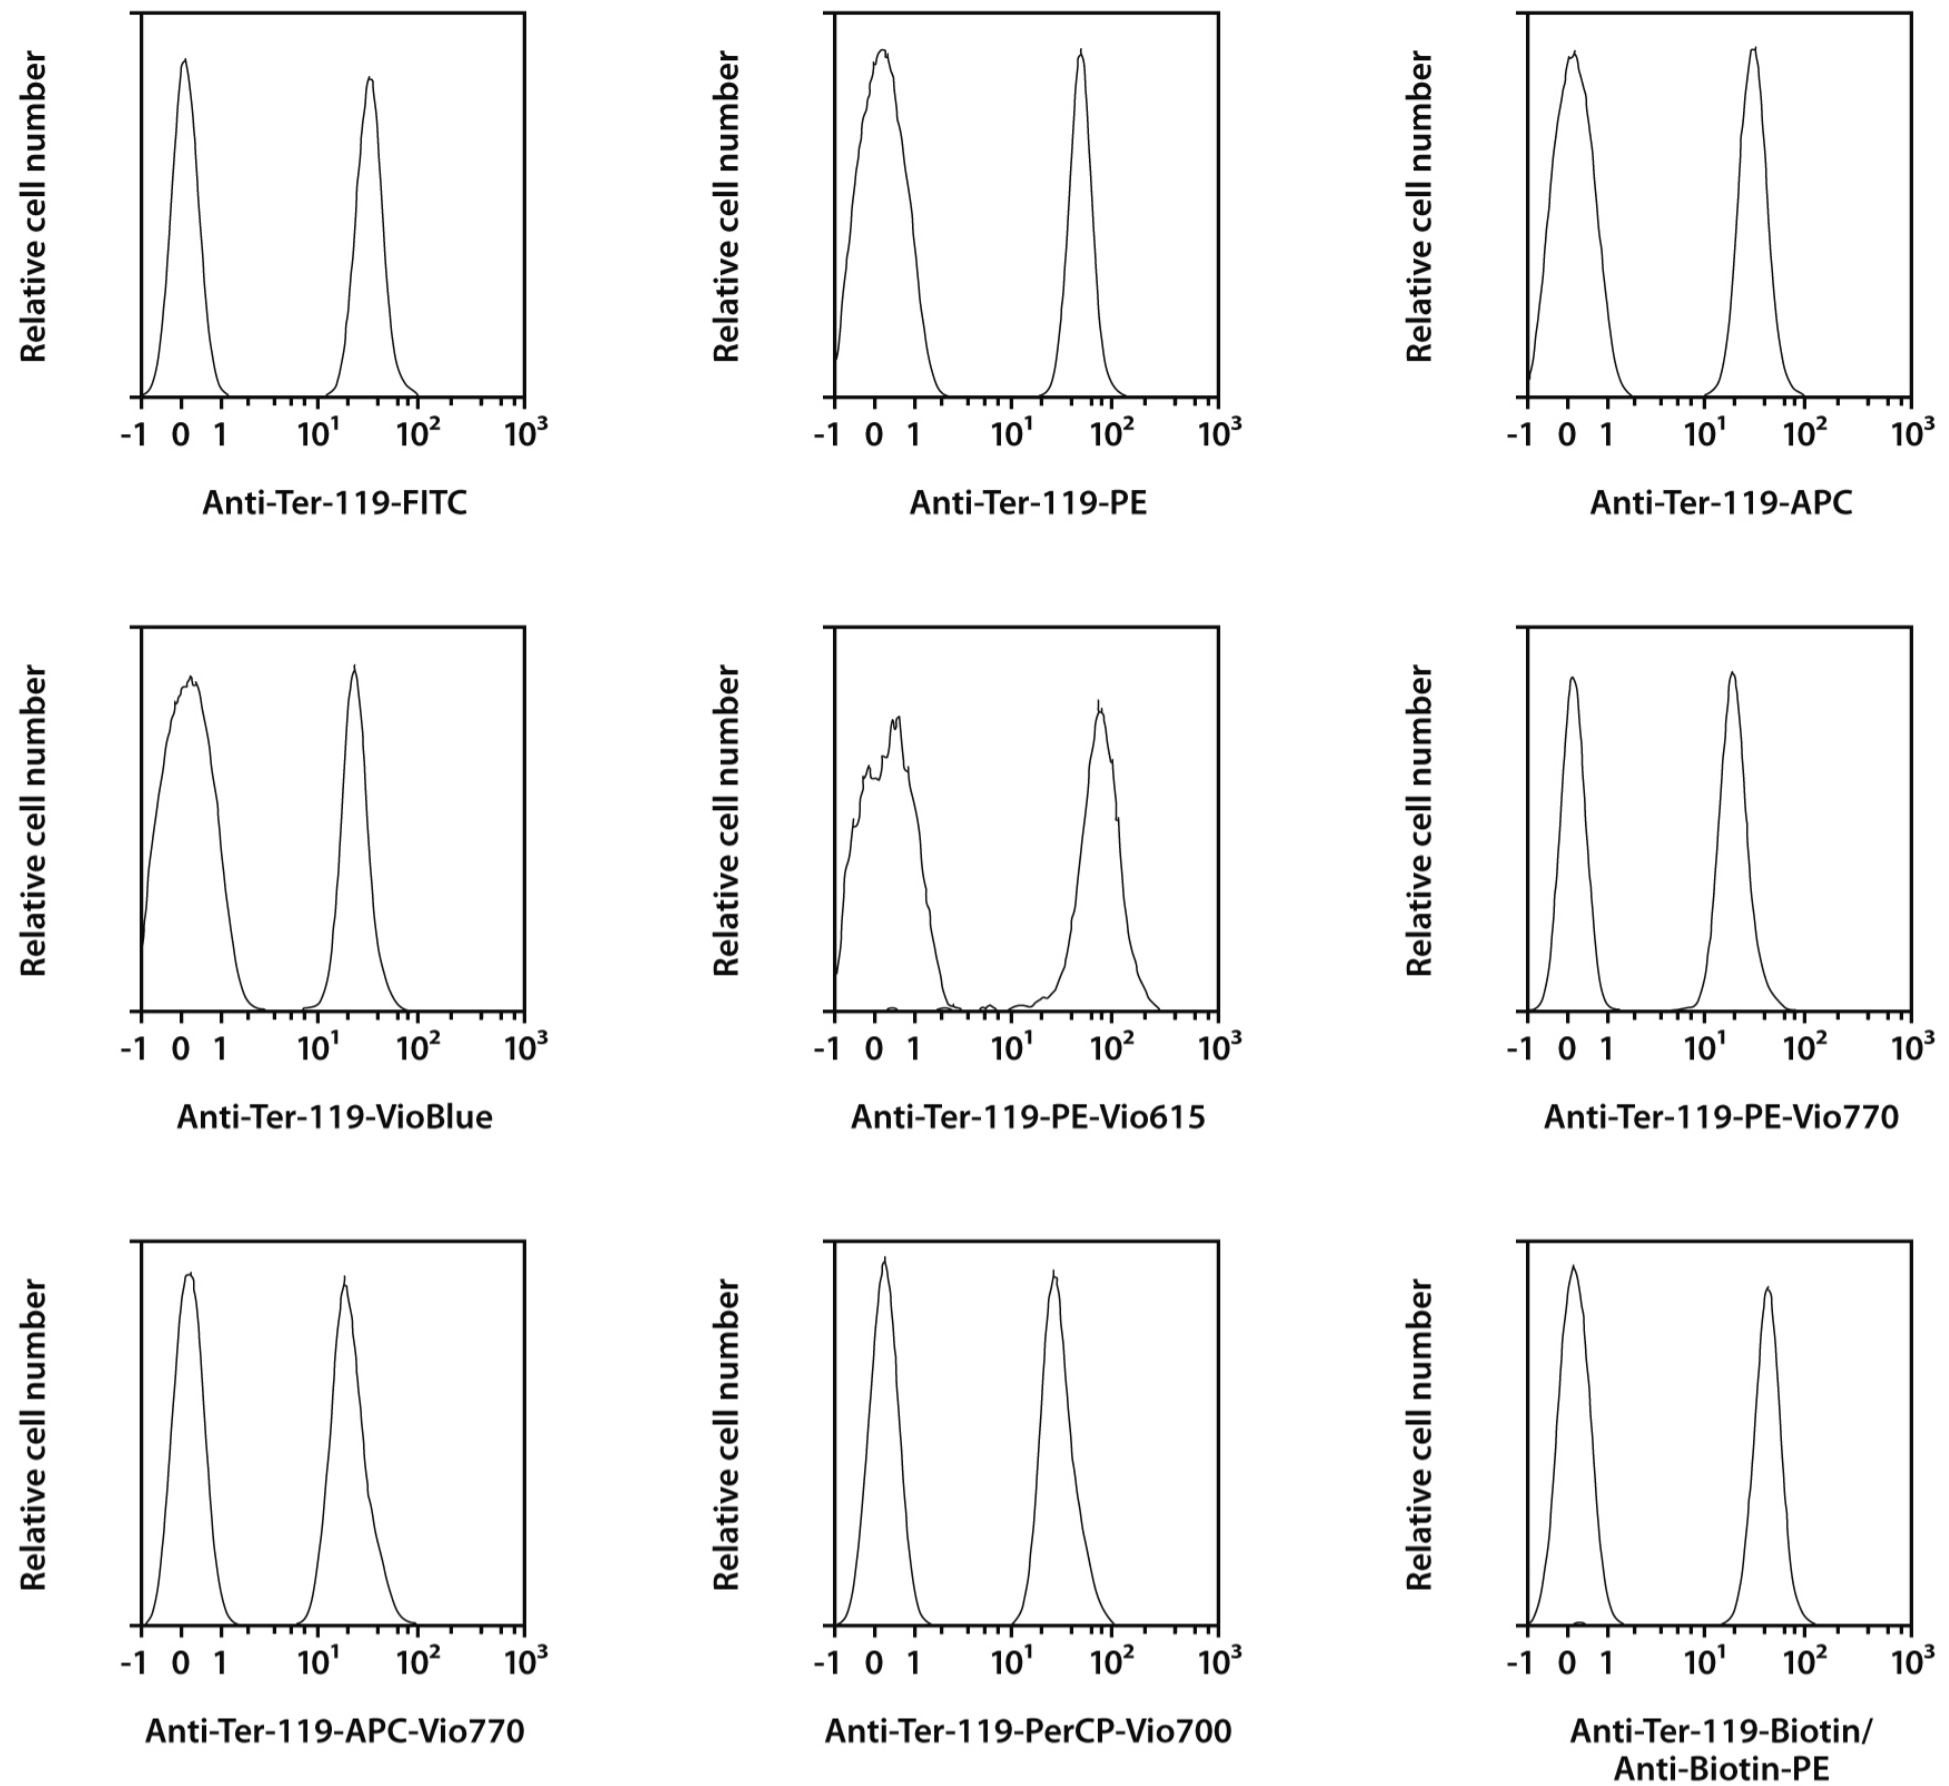

Warranty

The products sold hereunder are warranted only to be free from defects in workmanship and material at the time of delivery to the customer. Miltenyi Biotec GmbH makes no warranty or representation, either expressed or implied, with respect to the fitness of a product for a particular purpose. There are no warranties, expressed or implied, which extend beyond the technical specifications of the products. Miltenyi Biotec GmbH's liability is limited to either replacement of the products or refund of the purchase price. Miltenyi Biotec GmbH is not liable for any property damage, personal injury or economic loss caused by the product.

Miltenyi Biotec GmbH | Friedrich-Ebert-Straße 68 | 51429 Bergisch Gladbach | Germany | Phone +49 2204 8306-0 | Fax +49 2204 85197 | macs@miltenyibiotec.de | www.miltenyibiotec.com Miltenyi Biotec provides products and services worldwide. Visit www.miltenyibiotec.com/local to find your nearest Miltenyi Biotec contact.

Unless otherwise specifically indicated, Miltenyi Biotec products and services are for research use only and not for therapeutic or diagnostic use. autoMACS, MACS, MACSQuant, Vio, VioBlue, VioBright, and VioGreen are either trademarks or registered trademarks of Miltenyi Biotec GmbH. Copyright © 2016 Miltenyi Biotec GmbH. All rights reserved.